



CERTIFICATION by CUSTODIAN of RECORDS

Tucson Police Department Crime Laboratory
270 S. Stone Avenue Tucson, AZ 85701-1917

I hereby certify that these documents are a true and correct copy of the periodic maintenance* for the Intoxilyzer 8000 Serial Number 80-000323 maintained by the Tucson Police Department Crime Laboratory pursuant to the requirements of the Arizona Department of Public Safety for a quality assurance program.

TS4
2-10-2011

A quality assurance specialist (QAS) tested the instrument on the following dates. The acceptable accuracy limits, as defined in A.A.C. R13-10-104.A.2, for a 0.100AC solution are 0.090AC to 0.110AC.

Date: 02/10/2011 Cal 1 0.095 AC Cal 2 0.096 AC

Between the dates of 01/13/2011 and 02/10/2011 the instrument was operating properly and accurately.

The instrument was taken out of service for repair on N/A.
The instrument was returned to service on N/A.

Cheryl K. Straub

Cheryl K. Straub


02/10/2011

ADPS QAS Permit # 33408

SUBSCRIBED AND SWORN to before me this 10, day of February 20, 11.

A.M. Hernandez

Notary Public

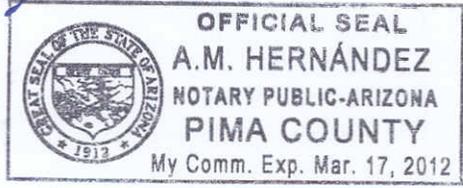

*Includes documents specified in A.A.C. R13-10-104.A.5

187cs

EXHIBIT G-4

THIS REPORT PREPARED PURSUANT TO DUTY IMPOSED BY
A.A.C. R13-10-104(A)

ARIZONA DEPARTMENT OF PUBLIC SAFETY

STANDARD QUALITY ASSURANCE PROCEDURES
INTOXILYZER MODEL 8000

STANDARD QUALITY ASSURANCE PROCEDURE

TS4
2.10.2011

QA SPECIALIST Cheryl Straub AGENCY Tucson Police Department
DATE 02/10/2011 TIME 09:57
INTOXILYZER SERIAL # 80-000323 LOCATION CRIME LAB

(✓) 1. Display reads "PUSH BUTTON TO START"

DIAGNOSTIC TESTS

- (✓) 1. Clock time check.
- (✓) 2. Date check.

OPERATIONAL TESTS

- (✓) 1. Alcohol-free subject test result 0. 000 AC.
- (✓) 2. Error recognition logic system functioning.
Not a Successfully Completed Test Sequence printed
- (✓) 3. Proper sample recognition system.
Not a Successfully Completed Test Sequence printed
Deficient sample printed.
- (✓) 4. Standard Calibration Check standard 0. 100 AC
Result: 0. 096 AC

Instrument is operating properly and accurately. YES NO

COMMENTS

SIGNATURE Cheryl Straub

Pursuant to section 28-1327, Arizona Revised Statutes, this document is a certified duplicate of the information contained in computer storage devices of the Tucson Police Department.

28 Feb

154

INTOXILYZER 8000
Location: TUCSON POLICE DEPT
Serial Number: 80-000323
02/10/2011 10:12:19

Standard Lot#: 642845
Last Changed By: C. STRAUB #50772

OAS: C. STRAUB #50772
TUCSON PD

| Test | g/210L | Time |
|-----------|--------|----------|
| Air Blank | 0.000 | 10:12:46 |
| Cal Check | 0.096 | 10:13:05 |
| Air Blank | 0.000 | 10:13:34 |



Operator's Signature

377
CS

B4

INTOXILYZER 8000
Location: TUCSON POLICE DEPT
Serial Number: 80-000323
02/10/2011 09:59:11

Standard Lot#: 642845
Last Changed By: C. STRAUB #50772

OAS: C. STRAUB #50772
TUCSON PD

Operator: C. STRAUB #50772
TUCSON PD

Subject: SOAP, SOAP
DOB: 11/11/1111
Sex: F Weight: 111

15 Minute Deprivation Period? Yes

| Test | g/210L | Time |
|-----------------|--------|----------|
| Air Blank | 0.000 | 10:00:06 |
| Diagnostic Test | Pass | 10:00:35 |
| Air Blank | 0.000 | 10:01:02 |
| 0.100 Cal Check | 0.095 | 10:01:21 |
| Air Blank | 0.000 | 10:01:51 |
| Subject Test | 0.000 | 10:02:24 |
| Air Blank | ABT* | 10:02:30 |
| Air Blank | 0.000 | 10:02:58 |

*Sequence Aborted

Not a Successfully
Completed
Test Sequence

477
CS

B4

INTOXILYZER 8000
Location: TUCSON POLICE DEPT
Serial Number: 80-000323
02/10/2011 10:03:10

Standard Lot#: 642845
Last Changed By: C. STRAUB #50772

OAS: C. STRAUB #50772
TUCSON PD

Operator: C. STRAUB #50772
TUCSON PD

Subject: SOAP, SOAP
DOB: 11/11/1111
Sex: F Weight: 111

15 Minute Deprivation Period? Yes

| Test | g/210L | Time |
|-----------|--------|----------|
| Air Blank | RFI* | 10:03:47 |
| Air Blank | IPS** | 10:03:57 |

*RFI Detect
**Improper Sample

Not a Successfully
Completed
Test Sequence

527 CS

154

INTOXILYZER 8000
Location: TUCSON POLICE DEPT
Serial Number: 80-000323
02/10/2011 10:04:12

Standard Lot#: 642845
Last Changed By: C. STRAUB #50772

DAS: C. STRAUB #50772
TUCSON PD

Operator: C. STRAUB #50772
TUCSON PD

Subject: SOAP, SOAP
DOB: 11/11/1111
Sex: F Weight: 111

15 Minute Deprivation Period? Yes

| Test | g/210L | Time |
|-----------------|--------|----------|
| Air Blank | 0.000 | 10:05:02 |
| Diagnostic Test | Pass | 10:05:31 |
| Air Blank | 0.000 | 10:05:58 |
| 0.100 Cal Check | 0.095 | 10:06:17 |
| Air Blank | 0.000 | 10:06:46 |
| Subject Test | 0.120* | 10:09:55 |
| Air Blank | 0.000 | 10:10:27 |
| Air Blank | 0.000 | 10:10:54 |
| Subject Test | XXX** | 10:11:14 |
| Air Blank | 0.000 | 10:11:47 |

*Deficient Sample
**Invalid Sample
Begin new deprivation period

Not a Successfully
Completed
Test Sequence

EXHIBIT G-2

687
CS

THIS REPORT PREPARED PURSUANT TO DUTY IMPOSED BY
A.A.C. R13-10-104(A)

ARIZONA DEPARTMENT OF PUBLIC SAFETY
STANDARD QUALITY ASSURANCE PROCEDURES
INTOXILYZER MODEL 8000
STANDARD CALIBRATION CHECK PROCEDURE

TS4
2.10.2011

QA Specialist Cheryl STRAUB AGENCY Tucson Police Department
DATE 02/10/2011 TIME 09:57
Intoxilyzer Serial # 80-000323 Location CRIME LAB

- (✓) 1. Ensure that gas tank is attached to instrument and contains a standard alcohol concentration solution 0. 100 AC.
OR
Pour a standard alcohol concentration solution N/A AC, into a clean dry simulator and assemble the simulator. Ensure that a tight seal has been made. Turn on the simulator and allow temperature to reach 34°C ± 0.2°C
- (✓) 2. Intoxilyzer 8000 display reads "PUSH BUTTON TO START"
- (✓) 3. Go to the "Control Testing Menu". Select "D" for dry control test or "W" for wet control test. After selection is made press ENTER.
- (✓) 4. Air blank completed.
- (✓) 5. Calibration check completed. Test results 0. 095 AC.
- (✓) 6. Air blank completed.
- (✓) 7. Remove printed record. Attach the record to the completed checklist.

SIGNATURE Cheryl Straub

Pursuant to section 28-1327, Arizona Revised Statutes, this document is a certified duplicate of the information contained in computer storage devices of the Tucson Police Department.

787
CS

134

INTOXILYZER 8000
Location: TUCSON POLICE DEPT
Serial Number: 80-000323
02/10/2011 09:57:36

Standard Lot#: 642845
Last Changed By: C. STRAUB #50772

OAS: C. STRAUB #50772
TUCSON PD

| Test | g/210L | Time |
|-----------|--------|----------|
| Air Blank | 0.000 | 09:58:03 |
| Cal Check | 0.095 | 09:58:22 |
| Air Blank | 0.000 | 09:58:51 |


Operator's Signature