



CERTIFICATION by CUSTODIAN of RECORDS

Tucson Police Department Crime Laboratory
1306 W. Miracle Mile, Tucson, AZ 85705

TS4
12-18-2015

I hereby certify that these documents are a true and correct copy of the periodic maintenance* for the Intoxilyzer 8000 Serial Number 80-000323 maintained by the Tucson Police Department Crime Laboratory pursuant to the requirements of the Arizona Department of Public Safety for a quality assurance program.

A quality assurance specialist (QAS) tested the instrument on the following dates. The acceptable accuracy limits, as defined in A.A.C. R13-10-104.A.2, for a 0.100AC solution are 0.090AC to 0.110AC.

Date: 12-10-15 Cal 1 0.102 AC Cal 2 0.102 AC

Between the dates of 11-12-15 and 12-10-15 the instrument was operating properly and accurately.

The instrument was taken out of service for repair on _____.
The instrument was returned to service on _____.


Amy L. Autret

12-16-15

ADPS QAS Permit # 33718

SUBSCRIBED AND SWORN to before me this 16, day of December, 20 15.

Notary Public

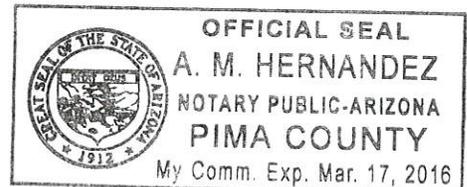

*Includes documents specified in A.A.C. R13-10-104.A.5

EXHIBIT G-4

THIS REPORT PREPARED PURSUANT TO DUTY IMPOSED BY
A.A.C. R13-10-104(A)

ARIZONA DEPARTMENT OF PUBLIC SAFETY
STANDARD QUALITY ASSURANCE PROCEDURES
INTOXILYZER MODEL 8000
STANDARD QUALITY ASSURANCE PROCEDURE

10F7
12.18.2015

QA SPECIALIST Amy Autret 53546 AGENCY Tucson Police Department

DATE 12-10-15 TIME 0851

INTOXILYZER SERIAL # 80-000323 LOCATION Laboratory

(✓) 1. Display reads "PUSH BUTTON TO START"

DIAGNOSTIC TESTS

- (✓) 1. Clock time check.
- (✓) 2. Date check.

OPERATIONAL TESTS

- (✓) 1. Alcohol-free subject test result 0. 000 AC.
- (✓) 2. Error recognition logic system functioning.
Not a Successfully Completed Test Sequence printed
- (✓) 3. Proper sample recognition system.
Not a Successfully Completed Test Sequence printed
Deficient sample printed.
- (✓) 4. Standard Calibration Check standard 0. 100 AC
Result: 0. 102 AC

Instrument is operating properly and accurately. YES NO

COMMENTS

SIGNATURE

INTOXILYZER 8000
Location: TUCSON POLICE DEPT
Serial Number: 80-000323
Core Version: 8105.48
12/10/2015 08:54:22

2 of 7
JLO
TS4

Standard Lot#: 12415100A4
Last Changed By: W. LOOMIS #53545

QAS: A. AUTRET #53546
TUCSON PD

Operator: A. AUTRET #53546
TUCSON PD

Subject: SQAP, SQAP
DOB: 11/11/1987
Sex: F Weight: 111

15 Minute Deprivation Period? Yes

Test	g/210L	Time
Air Blank	0.000	08:55:16
Diagnostic Test	Pass	08:55:50
Air Blank	0.000	08:56:17
0.100 Cal Check	0.103	08:56:38
Air Blank	0.000	08:57:08
Subject Test	0.000	08:57:25
Air Blank	0.000	08:57:53
Wait	ABT*	
Air Blank	0.000	08:58:27

*Sequence Aborted

Not a Successfully Completed Test Sequence

INTOXILYZER 8000
Location: TUCSON POLICE DEPT
Serial Number: 80-000323
Core Version: 8105.48
12/10/2015 08:58:43

3 of 7
JLD
TS4

Standard Lot#: 12415100A4
Last Changed By: W. LOOMIS #53545

QAS: A. AUTRET #53546
TUCSON PD

Operator: A. AUTRET #53546
TUCSON PD

Subject: SQAP, SQAP
DOB: 11/11/1987
Sex: F Weight: 111

15 Minute Deprivation Period? Yes

Test	g/210L	Time
Air Blank	0.000	08:59:33
Diagnostic Test	Pass	09:00:07
Air Blank	0.000	09:00:34
0.100 Cal Check	RFI*	09:00:48
Air Blank	IPS**	09:00:56

*RFI Detect
**Improper Sample

Not a Successfully Completed Test Sequence

Pursuant to section 28-1327, Arizona Revised Statutes, this document is a certified duplicate of the information contained in computer storage devices of the Tucson Police Department.

INTOXILYZER 8000
Location: TUCSON POLICE DEPT
Serial Number: 80-000323
Core Version: 8105.48
12/10/2015 09:01:01

4 of 7
JL
TBh

Standard Lot#: 12415100A4
Last Changed By: W. LOOMIS #53545

QAS: A. AUTRET #53546
TUCSON PD

Operator: A. AUTRET #53546
TUCSON PD

Subject: SQAP, SQAP
DOB: 11/11/1987
Sex: F Weight: 111

15 Minute Deprivation Period? Yes

Test	g/210L	Time
Air Blank	0.000	09:01:52
Diagnostic Test	Pass	09:02:27
Air Blank	0.000	09:02:54
0.100 Cal Check	0.102	09:03:15
Air Blank	0.000	09:03:44
Subject Test	0.208*	09:06:52
Air Blank	0.000	09:07:24
Air Blank	0.000	09:07:52
Subject Test	XXX**	09:08:12
Air Blank	0.000	09:08:46

*Deficient Sample

**Invalid Sample

Begin new deprivation period

Not a Successfully Completed Test Sequence

INTOXILYZER 8000

Location: TUCSON POLICE DEPT

Serial Number: 80-000323

Core Version: 8105.48

12/10/2015

09:09:04

Standard Lot#: 12415100A4

Last Changed By: W. LOOMIS #53545

QAS: A. AUTRET #53546

TUCSON PD

Operator: A. AUTRET #53546

TUCSON PD

Test	g/210L	Time
Air Blank	0.000	09:09:34
0.100 Cal Check	0.102	09:09:55
Air Blank	0.000	09:10:25

Preventative Maintenance
Performed -- Timer Reset

50F7
JL
Bh

EXHIBIT G-2

THIS REPORT PREPARED PURSUANT TO DUTY IMPOSED BY
A.A.C. R13-10-104(A)

ARIZONA DEPARTMENT OF PUBLIC SAFETY
STANDARD QUALITY ASSURANCE PROCEDURES
INTOXILYZER MODEL 8000
STANDARD CALIBRATION CHECK PROCEDURE

6 of 7
JLB
104
12-18-2015

QA Specialist Amy Autret 53546 AGENCY Tucson Police Department
DATE 12-10-15 TIME 0851
Intoxilyzer Serial # 80-000323 Location Laboratory

- (✓) 1. Ensure that gas tank is attached to instrument and contains a standard alcohol concentration solution 0. 100 AC.
OR
Pour a standard alcohol concentration solution _____ AC, into a clean dry simulator and assemble the simulator. Ensure that a tight seal has been made. Turn on the simulator and allow temperature to reach 34°C ± 0.2°C
- (✓) 2. Intoxilyzer 8000 display reads "PUSH BUTTON TO START"
- (✓) 3. Go to the "Control Testing Menu". Select "D" for dry control test or "W" for wet control test. After selection is made press ENTER.
- (✓) 4. Air blank completed.
- (✓) 5. Calibration check completed. Test results 0. 102 AC.
- (✓) 6. Air blank completed.
- (✓) 7. Remove printed record. Attach the record to the completed checklist.

SIGNATURE 

DPS Form Exh G-2 (Rev. 05-01)

INTOXILYZER 8000
Location: TUCSON POLICE DEPT
Serial Number: 80-000323
Core Version: 8105.48
12/10/2015 08:51:55

2 of 7
TS4
old

Standard Lot#: 12415100A4
Last Changed By: W. LOOMIS #53545

QAS: A. AUTRET #53546
TUCSON PD

Operator: A. AUTRET #53546
TUCSON PD

Test	g/210L	Time
Air Blank	0.000	08:52:25
0.100 Cal Check	0.102	08:52:46
Air Blank	0.000	08:53:15

Preventative Maintenance
Performed -- Timer Reset