



CERTIFICATION by CUSTODIAN of RECORDS

Tucson Police Department Crime Laboratory
1306 W. Miracle Mile, Tucson, AZ 85705

TSK
4.7.2016

I hereby certify that these documents are a true and correct copy of the periodic maintenance* for the Intoxilyzer 8000 Serial Number 80-000323 maintained by the Tucson Police Department Crime Laboratory pursuant to the requirements of the Arizona Department of Public Safety for a quality assurance program.

A quality assurance specialist (QAS) tested the instrument on the following dates. The acceptable accuracy limits, as defined in A.A.C. R13-10-104.A.2, for a 0.100AC solution are 0.090AC to 0.110AC.

Date: 3/31/2016 Cal 1 0.101 AC Cal 2 0.101 AC

Between the dates of 3/3/2016 and 3/31/2016 the instrument was operating properly and accurately.

The instrument was taken out of service for repair on
The instrument was returned to service on

William L Loomis

William L. Loomis


4/4/2016

ADPS QAS Permit # 33720

SUBSCRIBED AND SWORN to before me this 4th day of April, 2016.

Elma Escarcega

Notary Public

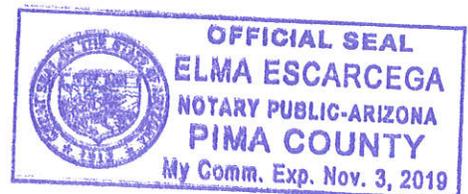

*Includes documents specified in A.A.C. R13-10-104.A.5

EXHIBIT G-4

THIS REPORT PREPARED PURSUANT TO DUTY IMPOSED BY
A.A.C. R13-10-104(A)

ARIZONA DEPARTMENT OF PUBLIC SAFETY

STANDARD QUALITY ASSURANCE PROCEDURES
INTOXILYZER MODEL 8000

STANDARD QUALITY ASSURANCE PROCEDURE

1 of 7
WLL
By
4-7-2016

QA SPECIALIST W. LOOMIS 53545 AGENCY Tucson Police Department

DATE 3/31/2016 TIME 14:49

INTOXILYZER SERIAL # 80-000323 LOCATION CRIME LAB

(✓) 1. Display reads "PUSH BUTTON TO START"

DIAGNOSTIC TESTS

- (✓) 1. Clock time check.
- (✓) 2. Date check.

OPERATIONAL TESTS

- (✓) 1. Alcohol-free subject test result 0. 000 AC.
- (✓) 2. Error recognition logic system functioning.
Not a Successfully Completed Test Sequence printed
- (✓) 3. Proper sample recognition system.
Not a Successfully Completed Test Sequence printed
Deficient sample printed.
- (✓) 4. Standard Calibration Check standard 0. 100 AC
Result: 0. 101 AC

Instrument is operating properly and accurately. YES NO

COMMENTS

SIGNATURE Willie Loomis

INTOXILYZER 8000
Location: TUCSON POLICE DEPT
Serial Number: 80-000323
Core Version: 8105.48
03/31/2016 14:50:55

2 of 7
WLL
BH

Standard Lot#: 12415100A4
Last Changed By: J. TRAINING #99999

QAS: W. LOOMIS #53545
TUCSON PD

Operator: W. LOOMIS #53545
TUCSON PD

Subject: SQAP, SQAP
DOB: 11/11/1987
Sex: M Weight: 222

15 Minute Deprivation Period? Yes

Test	g/210L	Time
Air Blank	0.000	14:52:20
Diagnostic Test	Pass	14:52:54
Air Blank	0.000	14:53:22
0.100 Cal Check	0.102	14:53:42
Air Blank	0.000	14:54:12
Subject Test	0.000	14:54:28
Air Blank	0.000	14:54:55
Wait	ABT*	
Air Blank	0.000	14:55:31

*Sequence Aborted

Not a Successfully Completed Test Sequence

Pursuant to section 28-1327, Arizona Revised Statutes, this document is a certified duplicate of the information contained in computer storage devices of the Tucson Police Department.

INTOXILYZER 8000
Location: TUCSON POLICE DEPT
Serial Number: 80-000323
Core Version: 8105.48
03/31/2016 14:56:06

Standard Lot#: 12415100A4
Last Changed By: J. TRAINING #99999

QAS: W. LOOMIS #53545
TUCSON PD

Operator: W. LOOMIS #53545
TUCSON PD

Subject: SQAP, SQAP
DOB: 11/11/1987
Sex: M Weight: 222

15 Minute Deprivation Period? Yes

Test	g/210L	Time
Air Blank	0.000	14:57:03
Diagnostic Test	Pass	14:57:37
Air Blank	0.000	14:58:05
0.100 Cal Check	RFI*	14:58:17
Air Blank	IPS**	14:58:29

*RFI Detect
**Improper Sample

3 of 7
WLL
TSH

Not a Successfully Completed Test Sequence

Pursuant to section 28-1327, Arizona Revised Statutes, this document is a certified duplicate of the information contained in computer storage devices of the Tucson Police Department.

INTOXILYZER 8000
Location: TUCSON POLICE DEPT
Serial Number: 80-000323
Core Version: 8105.48
03/31/2016 14:58:36

Standard Lot#: 12415100A4
Last Changed By: J. TRAINING #99999

QAS: W. LOOMIS #53545
TUCSON PD

Operator: W. LOOMIS #53545
TUCSON PD

Subject: SQAP, SQAP
DOB: 11/11/1987
Sex: M Weight: 222

15 Minute Deprivation Period? Yes

Test	g/210L	Time
Air Blank	0.000	15:00:05
Diagnostic Test	Pass	15:00:39
Air Blank	0.000	15:01:06
0.100 Cal Check	0.102	15:01:27
Air Blank	0.000	15:01:57
Subject Test	0.179*	15:05:04
Air Blank	0.000	15:05:37
Air Blank	0.000	15:06:05
Subject Test	XXX**	15:06:20
Air Blank	0.000	15:06:54

*Deficient Sample

**Invalid Sample

Begin new deprivation period

4 of 7
WLL
TBY

Not a Successfully Completed Test Sequence

INTOXILYZER 8000
Location: TUCSON POLICE DEPT
Serial Number: 80-000323
Core Version: 8105.48
03/31/2016 15:08:13

Standard Lot#: 12415100A4
Last Changed By: J. TRAINING #99999

QAS: W. LOOMIS #53545
TUCSON PD

Operator: W. LOOMIS #53545
TUCSON PD

Test	g/210L	Time
Air Blank	0.000	15:08:42
0.100 Cal Check	0.101	15:09:03
Air Blank	0.000	15:09:32

Preventative Maintenance
Performed -- Timer Reset

5 of 7
TBL WLL

EXHIBIT G-2

THIS REPORT PREPARED PURSUANT TO DUTY IMPOSED BY
A.A.C. R13-10-104(A)

ARIZONA DEPARTMENT OF PUBLIC SAFETY

STANDARD QUALITY ASSURANCE PROCEDURES
INTOXILYZER MODEL 8000

STANDARD CALIBRATION CHECK PROCEDURE

6 of 7
WLL
Tm
4-7-2016

QA Specialist W. LOOMIS 53545 AGENCY Tucson Police Department
DATE 3/31/2016 TIME 14:49
Intoxilyzer Serial # 80-000323 Location CRIME LAB

- (✓) 1. Ensure that gas tank is attached to instrument and contains a standard alcohol concentration solution 0. 100 AC.
OR
Pour a standard alcohol concentration solution _____ AC, into a clean dry simulator and assemble the simulator. Ensure that a tight seal has been made. Turn on the simulator and allow temperature to reach 34°C ± 0.2°C
- (✓) 2. Intoxilyzer 8000 display reads "PUSH BUTTON TO START"
- (✓) 3. Go to the "Control Testing Menu". Select "D" for dry control test or "W" for wet control test. After selection is made press ENTER.
- (✓) 4. Air blank completed.
- (✓) 5. Calibration check completed. Test results 0. 101 AC.
- (✓) 6. Air blank completed.
- (✓) 7. Remove printed record. Attach the record to the completed checklist.

SIGNATURE William Loomis

DPS Form Exh G-2 (Rev. 05-01)

INTOXILYZER 8000

Location: TUCSON POLICE DEPT

Serial Number: 80-000323

Core Version: 8105.48

03/31/2016

14:49:12

Standard Lot#: 12415100A4

Last Changed By: J. TRAINING #99999

QAS: W. LOOMIS #53545

TUCSON PD

Operator: W. LOOMIS #53545

TUCSON PD

Test g/210L Time

Air Blank 0.000 14:49:45
0.100 Cal Check 0.101 14:50:06
Air Blank 0.000 14:50:36

Preventative Maintenance
Performed -- Timer Reset

7 of 7
WLL
134