



CERTIFICATION by CUSTODIAN of RECORDS

Tucson Police Department Crime Laboratory
1306 W. Miracle Mile, Tucson, AZ 85705

By
7-29-2016

I hereby certify that these documents are a true and correct copy of the periodic maintenance* for the Intoxilyzer 8000 Serial Number 80-000332 maintained by the Tucson Police Department Crime Laboratory pursuant to the requirements of the Arizona Department of Public Safety for a quality assurance program.

A quality assurance specialist (QAS) tested the instrument on the following dates. The acceptable accuracy limits, as defined in A.A.C. R13-10-104.A.2, for a 0.100AC solution are 0.090AC to 0.110AC.

Date: 7-22-16 Cal 1 0.099 AC Cal 2 0.097 AC

Between the dates of and the instrument was operating properly and accurately.

The instrument was taken out of service for repair on
The instrument was returned to service on 7-22-16

[Handwritten signature of Amy L. Autret]

Amy L. Autret


7-26-16

ADPS QAS Permit # 33718

SUBSCRIBED AND SWORN to before me this 26th day of July, 2016.

[Handwritten signature of Elma Escarcega]

Notary Public

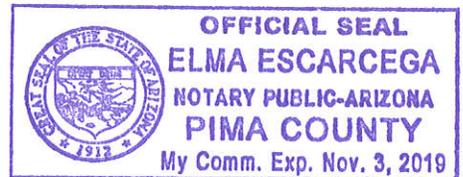

*Includes documents specified in A.A.C. R13-10-104.A.5



TUCSON POLICE DEPARTMENT
CRIME LABORATORY

INTOXILYZER SERVICE RECORD

10512
JLB

TJG
7-29-2016

QAS: Amy Autret 53546

Intoxilyzer Serial Number: 80-000332

Date Returned to Service: 7-22-16

EXHIBIT G-4

THIS REPORT PREPARED PURSUANT TO DUTY IMPOSED BY
A.A.C. R13-10-104(A)

ARIZONA DEPARTMENT OF PUBLIC SAFETY
STANDARD QUALITY ASSURANCE PROCEDURES
INTOXILYZER MODEL 8000
STANDARD QUALITY ASSURANCE PROCEDURE

2 of 12
JLB
TSL
7-29-2016

QA SPECIALIST Amy Autret 53546 AGENCY Tucson Police Department

DATE 7-22-16 TIME 1246

INTOXILYZER SERIAL # 80-000332 LOCATION Crime Laboratory

(✓) 1. Display reads "PUSH BUTTON TO START"

DIAGNOSTIC TESTS


- (✓) 1. Clock time check. 2 hours ahead - reset time
- (✓) 2. Date check.

OPERATIONAL TESTS

- (✓) 1. Alcohol-free subject test result 0. 000 AC.
- (✓) 2. Error recognition logic system functioning.
Not a Successfully Completed Test Sequence printed
- (✓) 3. Proper sample recognition system.
Not a Successfully Completed Test Sequence printed
Deficient sample printed.
- (✓) 4. Standard Calibration Check standard 0. 100 AC
Result: 0. 097 AC

Instrument is operating properly and accurately. YES NO

COMMENTS

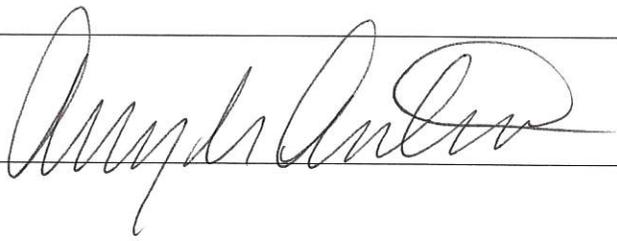SIGNATURE 

Pursuant to section 28-1327, Arizona Revised Statutes, this document is a certified duplicate of the information contained in computer storage devices of the Tucson Police Department.

INTOXILYZER 8000
Location:
Serial Number: 80-000332
Core Version: 8105.48
07/22/2016

12:51:50

3 of 12
JTB
TS4

Standard Lot#: 06616100A1
Last Changed By: A. AUTRET #53546

QAS: A. AUTRET #53546
TUCSON PD

Operator: A. AUTRET #53546
TUCSON PD

Subject: SQAP, SQAP
DOB: 11/11/1987
Sex: F Weight: 111

15 Minute Deprivation Period? Yes

Test	g/210L	Time
Air Blank	0.000	12:52:42
Diagnostic Test	Pass	12:53:17
Air Blank	0.000	12:53:45
0.100 Cal Check	0.098	12:54:05
Air Blank	0.000	12:54:35
Subject Test	0.000	12:54:54
Air Blank	0.000	12:55:21
Wait	ABT*	
Air Blank	0.000	12:56:01

*Sequence Aborted

Not a Successfully Completed Test Sequence

INTOXILYZER 8000
Location:
Serial Number: 80-000332
Core Version: 8105.48
07/22/2016

12:56:04

4 of 12
A
T84

Standard Lot#: 06616100A1
Last Changed By: A. AUTRET #53546

QAS: A. AUTRET #53546
TUCSON PD

Operator: A. AUTRET #53546
TUCSON PD

Subject: SQAP, SQAP
DOB: 11/11/1987
Sex: F Weight: 111

15 Minute Deprivation Period? Yes

Test	g/210L	Time
Air Blank	0.000	12:56:56
Diagnostic Test	Pass	12:57:31
Air Blank	0.000	12:57:58
0.100 Cal Check	RFI*	12:58:11
Air Blank	IPS**	12:58:21

*RFI Detect

**Improper Sample

Not a Successfully Completed Test Sequence

INTOXILYZER 8000
Location:
Serial Number: 80-000332
Core Version: 8105.48
07/22/2016 12:58:46

5 of 12
JL
TS4

Standard Lot#: 06616100A1
Last Changed By: A. AUTRET #53546

QAS: A. AUTRET #53546
TUCSON PD

Operator: A. AUTRET #53546
TUCSON PD

Subject: SQAP, SQAP
DOB: 11/11/1987
Sex: F Weight: 111

15 Minute Deprivation Period? Yes

Test	g/210L	Time
Air Blank	0.000	12:59:43
Diagnostic Test	Pass	13:00:18
Air Blank	0.000	13:00:45
0.100 Cal Check	0.098	13:01:06
Air Blank	0.000	13:01:36
Subject Test	0.241*	13:04:43
Air Blank	0.000	13:05:17
Air Blank	0.000	13:05:44
Subject Test	XXX**	13:06:08
Air Blank	0.000	13:06:43

*Deficient Sample

**Invalid Sample

Begin new deprivation period

Not a Successfully Completed Test Sequence

INTOXILYZER 8000

Location:

Serial Number: 80-000332

Core Version: 3105.40

07/22/2016

13:07:55

60512
Add
T84

Standard Lot#: 06616100A1

Last Changed By: A. AUTRET #53546

QAS: A. AUTRET #53546

TUCSON PD

Operator: A. AUTRET #53546

TUCSON PD

Test	g/210L	Time
Air Blank	0.000	13:08:24
0.100 Cal Check	0.097	13:08:45
Air Blank	0.000	13:09:15

Preventative Maintenance
Performed -- Timer Reset

EXHIBIT G-2

THIS REPORT PREPARED PURSUANT TO DUTY IMPOSED BY
A.A.C. R13-10-104(A)

7 of 12
TS4
7.29.2016

ARIZONA DEPARTMENT OF PUBLIC SAFETY

STANDARD QUALITY ASSURANCE PROCEDURES
INTOXILYZER MODEL 8000

STANDARD CALIBRATION CHECK PROCEDURE

QA Specialist Amy Autret 53546 AGENCY Tucson Police Department

DATE 7-22-16 TIME 1246

Intoxilyzer Serial # 80-000332 Location crime laboratory

- (✓) 1. Ensure that gas tank is attached to instrument and contains a standard alcohol concentration solution 0. 100 AC.
OR
Pour a standard alcohol concentration solution _____ AC, into a clean dry simulator and assemble the simulator. Ensure that a tight seal has been made. Turn on the simulator and allow temperature to reach 34°C ± 0.2°C
- (✓) 2. Intoxilyzer 8000 display reads "PUSH BUTTON TO START"
- (✓) 3. Go to the "Control Testing Menu". Select "D" for dry control test or "W" for wet control test. After selection is made press ENTER.
- (✓) 4. Air blank completed.
- (✓) 5. Calibration check completed. Test results 0. 099 AC.
- (✓) 6. Air blank completed.
- (✓) 7. Remove printed record. Attach the record to the completed checklist.

SIGNATURE



DPS Form Exh G-2 (Rev. 05-01)

INTOXILYZER 8000
Location:
Serial Number: 80-000332
Core Version: 8105.48
07/22/2016

12:46
14:46:28

80 of 12
JL
TS4

Standard Lot#: 06616100A1
Last Changed By: A. AUTRET #53546

QAS: A. AUTRET #53546
TUCSON PD

Operator: A. AUTRET #53546
TUCSON PD

Test	g/210L	Time
Air Blank	0.000	14:46:57
0.100 Cal Check	0.099	14:47:18
Air Blank	0.000	14:47:48

Preventative Maintenance
Performed -- Timer Reset



TUCSON POLICE DEPARTMENT
CRIME LABORATORY

9 of 12
JSD
TSB
7.29.2016

INTOXILYZER SERVICE RECORD
FOR
CALIBRATION GAS TANK CHANGE

Date: 7-22-16
QAS: Amy Autret 53546
Intoxilyzer Serial Number: 80-000332
New Lot Number: 06616100A1
New Expiration Date: 4-5-2018

- (✓) 1. Intoxilyzer 8000 display reads "PUSH BUTTON TO START"
- (✓) 2. Remove the old gas tank and install the new one.
- (✓) 3. Hit the "ESC" key twice and swipe the QAS card.
- (✓) 4. Go to the "M-Maintenance" menu and select "S-Standard Change."
Select "D" for dry gas and enter the following information:
Enter Target Value: 0.100
Enter Control Lot #: From the tank label
Enter Exp Date: From the tank label (mm/dd/yyyy)
Edit info Y/N? Y or N
Update Std Info? Y ENTER
"Please wait saving..."
- (✓) 5. Hit the "ESC" key twice.
- (✓) 6. Go to the "M-Maintenance" menu and select "T-Control Testing."
Select "D" for dry control test. After selection is made press ENTER.
- (✓) 7. Air blank completed.
- (✓) 8. Calibration check completed. Test results 0. 098 AC.
- (✓) 9. Air blank completed.
- (✓) 10. Remove printed record. Attach the record to the completed checklist.

SIGNATURE

INTOXILYZER 8000
Location:
Serial Number: 80-000332
Core Version: 8105.48
07/22/2016

12:41
14:41:04 *dlb*

10 of 12
dlb
By
7.29.2016

Standard Lot#: 06616100A1
Last Changed By: A. AUTRET #53546

QAS: #

Operator: A. AUTRET #53546
TUCSON PD

Test	g/210L	Time
Air Blank	0.000	14:41:37
0.100 Cal Check	0.098	14:41:58
Air Blank	0.000	14:42:28

Preventative Maintenance NOT
Performed -- Timer NOT Reset

Certificate of Calibration

12 of 12
dld
TS4

This is to certify the calibration of **Intoxilyzer**® serial number 80-000332, manufactured by CMI Inc., a subsidiary of MPD, Inc. of Owensboro, Kentucky, was tested and found to conform to the National Highway Traffic Safety Administration (NHTSA) Standard for Devices to Measure Breath Alcohol (Federal Register, Vol.58, No.179, pp 48705-48710, Sept. 17, 1993) for accuracy and precision. Reference materials are traceable through the National Institute of Standards and Technology (NIST) to the International System of Units (SI).

Date July 5, 2016 Signed [Signature]



Pursuant to Section 28.1327, Arizona Revised Statutes, this document is a certified duplicate of the information contained in computer storage devices of the Tucson Police Department.

316 East 9th Street
Owensboro, KY 42303
USA

Part No. 650517 Rev.A