



CERTIFICATION by CUSTODIAN of RECORDS

Tucson Police Department Crime Laboratory
1306 W. Miracle Mile, Tucson, AZ 85705

TS4
8.22.2016

I hereby certify that these documents are a true and correct copy of the periodic maintenance* for the Intoxilyzer 8000 Serial Number 80-000332 maintained by the Tucson Police Department Crime Laboratory pursuant to the requirements of the Arizona Department of Public Safety for a quality assurance program.

A quality assurance specialist (QAS) tested the instrument on the following dates. The acceptable accuracy limits, as defined in A.A.C. R13-10-104.A.2, for a 0.100AC solution are 0.090AC to 0.110AC.

Date: 8-19-16 Cal 1 0.099 AC Cal 2 0.096 AC

Between the dates of 7-22-16 and 8-19-16 the instrument was operating properly and accurately.

The instrument was taken out of service for repair on —.
The instrument was returned to service on —.

Amy L. Autret

Amy L. Autret

8-22-16

ADPS QAS Permit # 33718

SUBSCRIBED AND SWORN to before me this 22nd, day of August, 2016.

Elma Escarcega

Notary Public

*Includes documents specified in A.A.C. R13-10-104.A.5

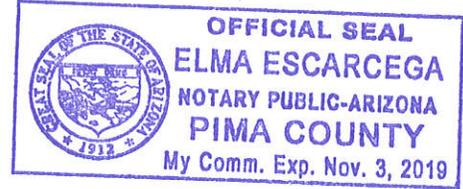


EXHIBIT G-4

THIS REPORT PREPARED PURSUANT TO DUTY IMPOSED BY
A.A.C. R13-10-104(A)

ARIZONA DEPARTMENT OF PUBLIC SAFETY
STANDARD QUALITY ASSURANCE PROCEDURES
INTOXILYZER MODEL 8000
STANDARD QUALITY ASSURANCE PROCEDURE

1 of 7
MLB
BSH 8.22.2016

QA SPECIALIST Amy Autret 53546 AGENCY Tucson Police Department

DATE 8-19-16 TIME 0813

INTOXILYZER SERIAL # 80-000332 LOCATION ODE

(✓) 1. Display reads "PUSH BUTTON TO START"

DIAGNOSTIC TESTS

- (✓) 1. Clock time check.
- (✓) 2. Date check.

OPERATIONAL TESTS

- (✓) 1. Alcohol-free subject test result 0. 000 AC.
- (✓) 2. Error recognition logic system functioning.
Not a Successfully Completed Test Sequence printed
- (✓) 3. Proper sample recognition system.
Not a Successfully Completed Test Sequence printed
Deficient sample printed.
- (✓) 4. Standard Calibration Check standard 0. 100 AC
Result: 0. 096 AC

Instrument is operating properly and accurately. YES NO

COMMENTS

SIGNATURE



INTOXILYZER 8000
Location:
Serial Number: 80-000332
Core Version: 8105.48
08/19/2016

08:18:28

2 of 7
@M
TSH

Standard Lot#: 06616100A1
Last Changed By: A. AUTRET #53546

QAS: A. AUTRET #53546
TUCSON PD

Operator: A. AUTRET #53546
TUCSON PD

Subject: SQAP, SQAP
DOB: 11/11/1987
Sex: F Weight: 111

15 Minute Deprivation Period? Yes

| Test | g/210L | Time |
|-----------------|--------|----------|
| Air Blank | 0.000 | 08:19:18 |
| Diagnostic Test | Pass | 08:19:53 |
| Air Blank | 0.000 | 08:20:20 |
| 0.100 Cal Check | 0.098 | 08:20:41 |
| Air Blank | 0.000 | 08:21:11 |
| Subject Test | 0.000 | 08:21:28 |
| Air Blank | 0.000 | 08:21:55 |
| Wait | ABT* | |
| Air Blank | 0.000 | 08:22:39 |

*Sequence Aborted

Not a Successfully Completed Test Sequence

INTOXILYZER 8000
Location:
Serial Number: 80-000332
Core Version: 8105.48
08/19/2016 08:23:00

3 of 7
dlt
Bh

Standard Lot#: 06616100A1
Last Changed By: A. AUTRET #53546

QAS: A. AUTRET #53546
TUCSON PD

Operator: A. AUTRET #53546
TUCSON PD

Subject: SQAP, SQAP
DOB: 11/11/1987
Sex: F Weight: 111

15 Minute Deprivation Period? Yes

| Test | g/210L | Time |
|-----------------|--------|----------|
| Air Blank | 0.000 | 08:23:54 |
| Diagnostic Test | Pass | 08:24:29 |
| Air Blank | 0.000 | 08:24:57 |
| 0.100 Cal Check | RFI* | 08:25:10 |
| Air Blank | IPS** | 08:25:18 |

*RFI Detect
**Improper Sample

Not a Successfully Completed Test Sequence

INTOXILYZER 8000
Location:
Serial Number: 80-000332
Core Version: 8105.48
08/19/2016

08:25:23

4 of 7
dlk
Bh

Standard Lot#: 06616100A1
Last Changed By: A. AUTRET #53546

QAS: A. AUTRET #53546
TUCSON PD

Operator: A. AUTRET #53546
TUCSON PD

Subject: SQAP, SQAP
DOB: 11/11/1987
Sex: F Weight: 111

15 Minute Deprivation Period? Yes

| Test | g/210L | Time |
|-----------------|--------|----------|
| Air Blank | 0.000 | 08:26:15 |
| Diagnostic Test | Pass | 08:26:50 |
| Air Blank | 0.000 | 08:27:18 |
| 0.100 Cal Check | 0.098 | 08:27:38 |
| Air Blank | 0.000 | 08:28:08 |
| Subject Test | 0.122* | 08:31:16 |
| Air Blank | 0.000 | 08:31:49 |
| Air Blank | 0.000 | 08:32:16 |
| Subject Test | XXX** | 08:32:46 |
| Air Blank | 0.000 | 08:33:20 |

*Deficient Sample

**Invalid Sample

Begin new deprivation period

Not a Successfully Completed Test Sequence

INTOXILYZER 8000

Location:

Serial Number: 80-000332

Core Version: 8105.48

08/19/2016

08:33:35

5 of 7
dB
BY

Standard Lot#: 06616100A1

Last Changed By: A. AUTRET #53546

QAS: A. AUTRET #53546

TUCSON PD

Operator: A. AUTRET #53546

TUCSON PD

| Test | g/210L | Time |
|-----------------|--------|----------|
| Air Blank | 0.000 | 08:34:05 |
| 0.100 Cal Check | 0.096 | 08:34:26 |
| Air Blank | 0.000 | 08:34:56 |

Preventative Maintenance
Performed -- Timer Reset

EXHIBIT G-2

THIS REPORT PREPARED PURSUANT TO DUTY IMPOSED BY
A.A.C. R13-10-104(A)

ARIZONA DEPARTMENT OF PUBLIC SAFETY

STANDARD QUALITY ASSURANCE PROCEDURES
INTOXILYZER MODEL 8000

STANDARD CALIBRATION CHECK PROCEDURE

6 of 7
all
BSH 8.22.2016

QA Specialist Amy Nutt + 53546 AGENCY Tucson Police Department
DATE 8-19-16 TIME 0813
Intoxilyzer Serial # 80-000332 Location ODE

- (✓) 1. Ensure that gas tank is attached to instrument and contains a standard alcohol concentration solution 0. 100 AC.
OR
Pour a standard alcohol concentration solution _____ AC, into a clean dry simulator and assemble the simulator. Ensure that a tight seal has been made. Turn on the simulator and allow temperature to reach 34°C ± 0.2°C
- (✓) 2. Intoxilyzer 8000 display reads "PUSH BUTTON TO START"
- (✓) 3. Go to the "Control Testing Menu". Select "D" for dry control test or "W" for wet control test. After selection is made press ENTER.
- (✓) 4. Air blank completed.
- (✓) 5. Calibration check completed. Test results 0. 099 AC.
- (✓) 6. Air blank completed.
- (✓) 7. Remove printed record. Attach the record to the completed checklist.

SIGNATURE



DPS Form Exh G-2 (Rev. 05-01)

