



CERTIFICATION by CUSTODIAN of RECORDS

Tucson Police Department Crime Laboratory
1306 W. Miracle Mile, Tucson, AZ 85705

TS4
11-25-2015

I hereby certify that these documents are a true and correct copy of the periodic maintenance* for the Intoxilyzer 8000 Serial Number 80-001108 maintained by the Tucson Police Department Crime Laboratory pursuant to the requirements of the Arizona Department of Public Safety for a quality assurance program.

A quality assurance specialist (QAS) tested the instrument on the following dates. The acceptable accuracy limits, as defined in A.A.C. R13-10-104.A.2, for a 0.100AC solution are 0.090AC to 0.110AC.

Date: 11/12/15 Cal 1 0.098 AC Cal 2 0.098 AC

Between the dates of 10/15/15 and 11/12/15 the instrument was operating properly and accurately.

The instrument was taken out of service for repair on _____.
The instrument was returned to service on _____.

[Signature]
Amy L. Autret


11/16/15

ADPS QAS Permit # 33718

SUBSCRIBED AND SWORN to before me this 16, day of November, 2015.

[Signature]

Notary Public

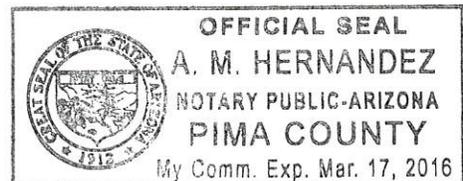

*Includes documents specified in A.A.C. R13-10-104.A.5

Pursuant to section 28-1327, Arizona Revised Statutes, this document is a certified duplicate of the information contained in computer storage devices of the Tucson Police Department.

EXHIBIT G-4

THIS REPORT PREPARED PURSUANT TO DUTY IMPOSED BY
A.A.C. R13-10-104(A)

ARIZONA DEPARTMENT OF PUBLIC SAFETY

STANDARD QUALITY ASSURANCE PROCEDURES
INTOXILYZER MODEL 8000

STANDARD QUALITY ASSURANCE PROCEDURE

10 of 7
JSH
11-25-2015

QA SPECIALIST Amy Antret 53546 AGENCY Tucson Police Department

DATE 11/12/15 TIME 0800

INTOXILYZER SERIAL # 80-001108 LOCATION Lab

(✓) 1. Display reads "PUSH BUTTON TO START"

DIAGNOSTIC TESTS

- (✓) 1. Clock time check.
- (✓) 2. Date check.


OPERATIONAL TESTS

- (✓) 1. Alcohol-free subject test result 0. 000 AC.
- (✓) 2. Error recognition logic system functioning.
Not a Successfully Completed Test Sequence printed
- (✓) 3. Proper sample recognition system.
Not a Successfully Completed Test Sequence printed
Deficient sample printed.
- (✓) 4. Standard Calibration Check standard 0. 100 AC
Result: 0. 098 AC

Instrument is operating properly and accurately. YES NO

COMMENTS

SIGNATURE

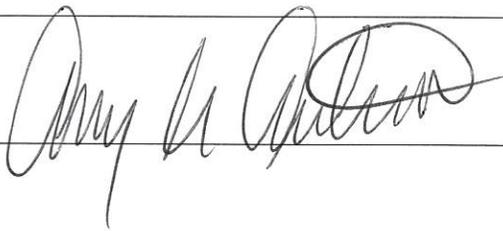

INTOXILYZER 8000
Location: TUCSON PD
Serial Number: 80-001108
Core Version: 8105.48
11/12/2015

08:02:24

20F7
JL
754

Standard Lot#: 12415100A4
Last Changed By: W. LOOMIS #53545

QAS: A. AUTRET #53546
TUCSON PD

Operator: A. AUTRET #53546
TUCSON PD

Subject: SQAP, SQAP
DOB: 11/11/1987
Sex: F Weight: 111

15 Minute Deprivation Period? Yes

Test	g/210L	Time
Air Blank	0.000	08:03:18
Diagnostic Test	Pass	08:03:53
Air Blank	0.000	08:04:20
0.100 Cal Check	0.099	08:04:41
Air Blank	0.000	08:05:10
Subject Test	0.000	08:05:30
Air Blank	0.000	08:05:58
Wait	ABT*	
Air Blank	0.000	08:06:35

*Sequence Aborted

Not a Successfully Completed Test Sequence

Pursuant to section 28-1327, Arizona Revised Statutes, this document is a certified duplicate of the information contained in computer storage devices of the Tucson Police Department.

INTOXILYZER 8000
Location: TUCSON PD
Serial Number: 80-001108
Core Version: 8105.48
11/12/2015

08:06:57

3057
dlb
TS4

Standard Lot#: 12415100A4
Last Changed By: W. LOOMIS #53545

QAS: A. AUTRET #53546
TUCSON PD

Operator: A. AUTRET #53546
TUCSON PD

Subject: SQAP, SQAP
DOB: 11/11/1987
Sex: F Weight: 111

15 Minute Deprivation Period? Yes

Test	g/210L	Time
Air Blank	0.000	08:07:49
Diagnostic Test	Pass	08:08:24
Air Blank	0.000	08:08:52
0.100 Cal Check	RFI*	08:09:07
Air Blank	IPS**	08:09:14

*RFI Detect

**Improper Sample

Not a Successfully Completed Test Sequence

Pursuant to section 28-1327, Arizona Revised Statutes, this document is a certified duplicate of the information contained in computer storage devices of the Tucson Police Department.

INTOXILYZER 8000
Location: TUCSON PD
Serial Number: 80-001108
Core Version: 8105.48
11/12/2015

08:09:37

4 of 7
JL
TS4

Standard Lot#: 12415100A4
Last Changed By: W. LOOMIS #53545

QAS: A. AUTRET #53546
TUCSON PD

Operator: A. AUTRET #53546
TUCSON PD

Subject: SQAP, SQAP
DOB: 11/11/1987
Sex: F Weight: 111

15 Minute Deprivation Period? Yes

Test	g/210L	Time
Air Blank	0.000	08:10:29
Diagnostic Test	Pass	08:11:04
Air Blank	0.000	08:11:32
0.100 Cal Check	0.098	08:11:52
Air Blank	0.000	08:12:22
Subject Test	0.092*	08:15:29
Air Blank	0.000	08:16:02
Air Blank	0.000	08:16:29
Subject Test	XXX**	08:16:56
Air Blank	0.000	08:17:30

*Deficient Sample

**Invalid Sample

Begin new deprivation period

Not a Successfully Completed Test Sequence

INTOXILYZER 8000
Location: TUCSON PD
Serial Number: 80-001108
Core Version: 8105.48
11/12/2015 08:17:47

5 of 7
JW
TS4

Standard Lot#: 12415100A4
Last Changed By: W. LOOMIS #53545

QAS: A. AUTRET #53546
TUCSON PD

Operator: A. AUTRET #53546
TUCSON PD

Test	g/210L	Time
Air Blank	0.000	08:18:17
0.100 Cal Check	0.098	08:18:38
Air Blank	0.000	08:19:07

Preventative Maintenance
Performed -- Timer Reset

EXHIBIT G-2

THIS REPORT PREPARED PURSUANT TO DUTY IMPOSED BY
A.A.C. R13-10-104(A)

ARIZONA DEPARTMENT OF PUBLIC SAFETY

STANDARD QUALITY ASSURANCE PROCEDURES
INTOXILYZER MODEL 8000

STANDARD CALIBRATION CHECK PROCEDURE

6 of 7
JLB

TS4
11-25-2015

QA Specialist Amy Autret 53546 AGENCY Tucson Police Department
DATE 11/12/15 TIME 0800
Intoxilyzer Serial # 80-001108 Location Lab

- (✓) 1. Ensure that gas tank is attached to instrument and contains a standard alcohol concentration solution 0. 100 AC.
OR
Pour a standard alcohol concentration solution _____ AC, into a clean dry simulator and assemble the simulator. Ensure that a tight seal has been made. Turn on the simulator and allow temperature to reach 34°C ± 0.2°C.
- (✓) 2. Intoxilyzer 8000 display reads "PUSH BUTTON TO START"
- (✓) 3. Go to the "Control Testing Menu". Select "D" for dry control test or "W" for wet control test. After selection is made press ENTER.
- (✓) 4. Air blank completed.
- (✓) 5. Calibration check completed. Test results 0. 098 AC.
- (✓) 6. Air blank completed.
- (✓) 7. Remove printed record. Attach the record to the completed checklist.

SIGNATURE 

DPS Form Exh G-2 (Rev. 05-01)

INTOXILYZER 8000
Location: TUCSON PD
Serial Number: 80-001108
Core Version: 8105.48
11/12/2015 08:00:00

7087
TS4

Standard Lot#: 12415100A4
Last Changed By: W. LOOMIS #53545

QAS: A. AUTRET #53546
TUCSON PD

Operator: A. AUTRET #53546
TUCSON PD

Test	g/210L	Time
Air Blank	0.000	08:00:30
0.100 Cal Check	0.098	08:00:51
Air Blank	0.000	08:01:20

Preventative Maintenance
Performed -- Timer Reset