



CERTIFICATION by CUSTODIAN of RECORDS

Tucson Police Department Crime Laboratory
1306 W. Miracle Mile, Tucson, AZ 85705

TS4
8-22-2016

I hereby certify that these documents are a true and correct copy of the periodic maintenance* for the Intoxilyzer 8000 Serial Number 80-001163 maintained by the Tucson Police Department Crime Laboratory pursuant to the requirements of the Arizona Department of Public Safety for a quality assurance program.

A quality assurance specialist (QAS) tested the instrument on the following dates. The acceptable accuracy limits, as defined in A.A.C. R13-10-104.A.2, for a 0.100AC solution are 0.090AC to 0.110AC.

Date: 8/18/2016 Cal 1 0.096 AC Cal 2 0.096 AC

Between the dates of 7/22/2016 and 8/18/2016 the instrument was operating properly and accurately.

The instrument was taken out of service for repair on _____.
The instrument was returned to service on _____.

William L Loomis

William L. Loomis


8/22/2016

ADPS QAS Permit # 33720

SUBSCRIBED AND SWORN to before me this 22nd, day of August, 2016.

Elma Escarcega

Notary Public

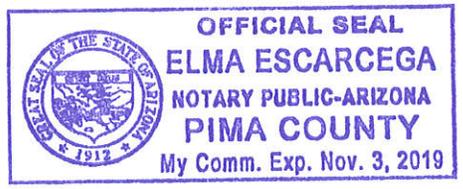

*Includes documents specified in A.A.C. R13-10-104.A.5

EXHIBIT G-4

THIS REPORT PREPARED PURSUANT TO DUTY IMPOSED BY
A.A.C. R13-10-104(A)

ARIZONA DEPARTMENT OF PUBLIC SAFETY

STANDARD QUALITY ASSURANCE PROCEDURES
INTOXILYZER MODEL 8000

STANDARD QUALITY ASSURANCE PROCEDURE

1 of 7
WLL
TJh 8.22.2016

QA SPECIALIST W. LOOMIS 53545 AGENCY Tucson Police Department

DATE 8/18/2016 TIME 12:22

INTOXILYZER SERIAL # 80-001163 LOCATION CRIME LAB

(✓) 1. Display reads "PUSH BUTTON TO START"

DIAGNOSTIC TESTS

- (✓) 1. Clock time check.
- (✓) 2. Date check.

OPERATIONAL TESTS

- (✓) 1. Alcohol-free subject test result 0. 000 AC.
- (✓) 2. Error recognition logic system functioning.
Not a Successfully Completed Test Sequence printed
- (✓) 3. Proper sample recognition system.
Not a Successfully Completed Test Sequence printed
Deficient sample printed.
- (✓) 4. Standard Calibration Check standard 0. 100 AC
Result: 0. 096 AC

Instrument is operating properly and accurately. YES NO

COMMENTS

SIGNATURE

Will Loomis

3 of 7
WLL
TS4

INTOXILYZER 8000
Location: TUCSON POLICE DEPT
Serial Number: 80-001163
Core Version: 8105.48
08/18/2016 12:29:54

Standard Lot#: 15615100A1
Last Changed By: T. GALLEGOS #28847

OAS: W. LOOMIS #53545
TUCSON PD

Operator: W. LOOMIS #53545
TUCSON PD

Subject: SOAP, SOAP
DOB: 11/11/1987
Sex: M Weight: 222

15 Minute Deprivation Period? Yes

Test	g/210L	Time
Air Blank	0.000	12:31:12
Diagnostic Test	Pass	12:31:50
Air Blank	0.000	12:32:17
0.100 Cal Check	RFI*	12:32:37
Air Blank	IPS**	12:32:46

*RFI Detect
**Improper Sample

Not a Successfully
Completed
Test Sequence

2 of 7
WLL
Dh

INTOXILYZER 8000
Location: TUCSON POLICE DEPT
Serial Number: 80-001163
Core Version: 8105.48
08/18/2016 12:25:04

Standard Lot#: 15615100A1
Last Changed By: T. GALLEGOS #28847

OAS: W. LOOMIS #53545
TUCSON PD

Operator: W. LOOMIS #53545
TUCSON PD

Subject: SQAP,SQAP
DOB: 11/11/1987
Sex: M Weight: 222

15 Minute Deprivation Period? Yes

Test	g/210L	Time
Air Blank	0.000	12:26:24
Diagnostic Test	Pass	12:27:02
Air Blank	0.000	12:27:29
0.100 Cal Check	0.095	12:27:50
Air Blank	0.000	12:28:19
Subject Test	0.000	12:28:42
Air Blank	0.000	12:29:09
Wait	ABT*	
Air Blank	0.000	12:29:44

*Sequence Aborted

Not a Successfully
Completed
Test Sequence

INTOXILYZER 8000
Location: TUCSON POLICE DEPT
Serial Number: 80-001163
Core Version: 8105.48
08/18/2016 12:33:16

4 of 7
Tsu
WLL

Standard Lot#: 15615100A1
Last Changed By: T. GALLEGOS #28847

OAS: W. LOOMIS #53545
TUCSON PD

Operator: W. LOOMIS #53545
TUCSON PD

Subject: SOAP, SOAP
DOB: 11/11/1987
Sex: M Weight: 222

15 Minute Deprivation Period? Yes

Test	g/210L	Time
Air Blank	0.000	12:34:35
Diagnostic Test	Pass	12:35:13
Air Blank	0.000	12:35:40
0.100 Cal Check	0.095	12:36:01
Air Blank	0.000	12:36:30
Subject Test	0.064*	12:39:38
Air Blank	0.000	12:40:10
Air Blank	0.000	12:40:37
Subject Test	XXX**	12:41:01
Air Blank	0.000	12:41:34

*Deficient Sample

**Invalid Sample

Begin new deprivation period

Not a Successfully
Completed
Test Sequence

5 of 7
0 WLL
Bk

INTOXILYZER 8000
Location: TUCSON POLICE DEPT
Serial Number: 81-001163
Core Version: 8105.48
08/18/2016 12:42:14

Standard Lot#: 15615100A1
Last Changed By: T. GALLEGOS #28847

OAS: W. LOOMIS #53545
TUCSON PD

Operator: W. LOOMIS #53545
TUCSON PD

Test	g/210L	Time
Air Blank	0.000	12:42:44
0.100 Cal Check	0.096	12:43:05
Air Blank	0.000	12:43:35

Preventative Maintenance
Performed -- Timer Reset

EXHIBIT G-2

THIS REPORT PREPARED PURSUANT TO DUTY IMPOSED BY
A.A.C. R13-10-104(A)

ARIZONA DEPARTMENT OF PUBLIC SAFETY
STANDARD QUALITY ASSURANCE PROCEDURES
INTOXILYZER MODEL 8000

STANDARD CALIBRATION CHECK PROCEDURE

6 of 7
WLL
TS4
8.22.2016

QA Specialist W. LOOMIS 53545 AGENCY Tucson Police Department
DATE 8/18/2016 TIME 12:22
Intoxilyzer Serial # 80-001163 Location CRIME LAB

- (✓) 1. Ensure that gas tank is attached to instrument and contains a standard alcohol concentration solution 0. 100 AC.
OR
Pour a standard alcohol concentration solution _____ AC, into a clean dry simulator and assemble the simulator. Ensure that a tight seal has been made. Turn on the simulator and allow temperature to reach 34°C ± 0.2°C
- (✓) 2. Intoxilyzer 8000 display reads "PUSH BUTTON TO START"
- (✓) 3. Go to the "Control Testing Menu". Select "D" for dry control test or "W" for wet control test. After selection is made press ENTER.
- (✓) 4. Air blank completed.
- (✓) 5. Calibration check completed. Test results 0. 096 AC.
- (✓) 6. Air blank completed.
- (✓) 7. Remove printed record. Attach the record to the completed checklist.

SIGNATURE Will Loomis

INTOXILYZER 8000
Location: TUCSON POLICE DEPT
Serial Number: 80-001163
Core Version: 8105.48
08/18/2016 12:22:11

Standard Lot#: 15615100A1
Last Changed By: T. GALLEGOS #28847

QAS: W. LOOMIS #53545
TUCSON PD

Operator: W. LOOMIS #53545
TUCSON PD

Test	g/210L	Time
Air Blank	0.000	12:22:40
0.100 Cal Check	0.096	12:23:01
Air Blank	0.000	12:23:31

Preventative Maintenance
Performed -- Timer Reset

7 of 7
WLL
Bh