



CERTIFICATION by CUSTODIAN of RECORDS
 Tucson Police Department Crime Laboratory
 1306 W. Miracle Mile, Tucson, AZ 85705

TS4
 12-3-2013

I hereby certify that these documents are a true and correct copy of the periodic maintenance* for the Intoxilyzer 8000 Serial Number 80-002201 maintained by the Tucson Police Department Crime Laboratory pursuant to the requirements of the Arizona Department of Public Safety for a quality assurance program.

A quality assurance specialist (QAS) tested the instrument on the following dates. The acceptable accuracy limits, as defined in A.A.C. R13-10-104.A.2, for a 0.100AC solution are 0.090AC to 0.110AC.

Date: 11/8/13 Cal 1 0.100 AC Cal 2 0.099 AC

Between the dates of 10/11/13 and 11/8/13 the instrument was operating properly and accurately.


The instrument was taken out of service for repair on -.
 The instrument was returned to service on -.

Sarah Cione
 Sarah L. Cione

11/20/13
 ADPS QAS Permit # 33355

SUBSCRIBED AND SWORN to before me this 20th day of November, 2013.

Elma Escarcega
 Notary Public

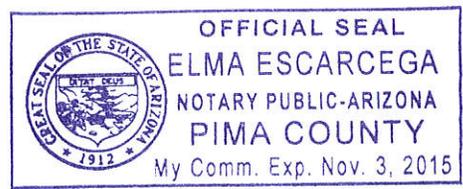

*Includes documents specified in A.A.C. R13-10-104.A.5

EXHIBIT G-4

THIS REPORT PREPARED PURSUANT TO DUTY IMPOSED BY
A.A.C. R13-10-104(A)

1 of 7
sc
TSK
12.3.2013

ARIZONA DEPARTMENT OF PUBLIC SAFETY

STANDARD QUALITY ASSURANCE PROCEDURES
INTOXILYZER MODEL 8000

STANDARD QUALITY ASSURANCE PROCEDURE

QA SPECIALIST Sarah Cione AGENCY Tucson Police Department

DATE 11/8/13 TIME 1257

INTOXILYZER SERIAL # 80-002201 LOCATION Crime Lab

() 1. Display reads "PUSH BUTTON TO START"

DIAGNOSTIC TESTS

- () 1. Clock time check.
- () 2. Date check.

OPERATIONAL TESTS

- () 1. Alcohol-free subject test result 0. 000 AC.
- () 2. Error recognition logic system functioning.
Not a Successfully Completed Test Sequence printed
- () 3. Proper sample recognition system.
Not a Successfully Completed Test Sequence printed
Deficient sample printed.
- () 4. Standard Calibration Check standard 0. 100 AC
Result: 0. 099 AC

Instrument is operating properly and accurately. YES NO

COMMENTS

SIGNATURE Sarah Cione

INTOXILYZER 8000
Location: TUCSON PD
Serial Number: 80-002201
Core Version: 8105.48
11/08/2013

12:59:57

2 of 7
sc
TBH

Standard Lot#: 30412100A1
Last Changed By: R. SZELEWSKI #46927

QAS: S. CIONE #50616
TUCSON PD

Operator: S. CIONE #50616
TUCSON PD

Subject: SQAP, SQAP
DOB: 11/11/1980
Sex: F Weight: 111

15 Minute Deprivation Period? Yes

Test	g/210L	Time
Air Blank	0.000	13:00:40
Diagnostic Test	Pass	13:01:15
Air Blank	0.000	13:01:43
0.100 Cal Check	0.100	13:02:03
Air Blank	0.000	13:02:33
Subject Test	0.000	13:02:59
Air Blank	0.000	13:03:26
Wait	ABT*	
Air Blank	0.000	13:04:01

*Sequence Aborted

Not a Successfully Completed Test Sequence

INTOXILYZER 8000
Location: TUCSON PD
Serial Number: 80-002201
Core Version: 8105.48
11/08/2013

13:04:42

3 of 7
BH SC

Standard Lot#: 30412100A1
Last Changed By: R. SZELEWSKI #46927

QAS: S. CIONE #50616
TUCSON PD

Operator: S. CIONE #50616
TUCSON PD

Subject: SQAP, SQAP
DOB: 11/11/1980
Sex: F Weight: 111

15 Minute Deprivation Period? Yes

Test	g/210L	Time
Air Blank	0.000	13:05:42
Diagnostic Test	Pass	13:06:17
Air Blank	0.000	13:06:45
0.100 Cal Check	RFI*	13:07:05
Air Blank	IPS**	13:07:16

*RFI Detect

**Improper Sample

Not a Successfully Completed Test Sequence

INTOXILYZER 8000
Location: TUCSON PD
Serial Number: 80-002201
Core Version: 8105.48
11/08/2013

13:07:26

4 of 7_{sc}
186

Standard Lot#: 30412100A1
Last Changed By: R. SZELEWSKI #46927

QAS: S. CIONE #50616
TUCSON PD

Operator: S. CIONE #50616
TUCSON PD

Subject: SQAP, SQAP
DOB: 11/11/1980
Sex: F Weight: 111

15 Minute Deprivation Period? Yes

Test	g/210L	Time
Air Blank	0.000	13:08:17
Diagnostic Test	Pass	13:08:52
Air Blank	0.000	13:09:19
0.100 Cal Check	0.100	13:09:40
Air Blank	0.000	13:10:09
Subject Test	0.274*	13:13:17
Air Blank	0.000	13:13:50
Air Blank	0.000	13:14:17
Subject Test	XXX**	13:14:29
Air Blank	0.000	13:15:03

*Deficient Sample

**Invalid Sample

Begin new deprivation period

Not a Successfully Completed Test Sequence

INTOXILYZER 8000
Location: TUCSON PD
Serial Number: 80-002201
Core Version: 8105.48
11/08/2013 13:15:14

5 of 7
TS4 SC

Standard Lot#: 30412100A1
Last Changed By: R. SZELEWSKI #46927

QAS: S. CIONE #50616
TUCSON PD

Operator: S. CIONE #50616
TUCSON PD

Test	g/210L	Time
Air Blank	0.000	13:15:42
0.100 Cal Check	0.099	13:16:03
Air Blank	0.000	13:16:33

Preventative Maintenance
Performed -- Timer Reset

EXHIBIT G-2

THIS REPORT PREPARED PURSUANT TO DUTY IMPOSED BY
A.A.C. R13-10-104(A)

ARIZONA DEPARTMENT OF PUBLIC SAFETY
STANDARD QUALITY ASSURANCE PROCEDURES
INTOXILYZER MODEL 8000
STANDARD CALIBRATION CHECK PROCEDURE

607
SC
TS4
12.3.2013

QA Specialist Sarah Cione AGENCY Tucson Police Department
DATE 11/8/13 TIME 1257
Intoxilyzer Serial # 80-002201 Location Crime Lab

- (✓) 1. Ensure that gas tank is attached to instrument and contains a standard alcohol concentration solution 0. 100 AC.
OR
Pour a standard alcohol concentration solution _____ AC, into a clean dry simulator and assemble the simulator. Ensure that a tight seal has been made. Turn on the simulator and allow temperature to reach 34°C ± 0.2°C
- (✓) 2. Intoxilyzer 8000 display reads "PUSH BUTTON TO START"
- (✓) 3. Go to the "Control Testing Menu". Select "D" for dry control test or "W" for wet control test. After selection is made press ENTER.
- (✓) 4. Air blank completed.
- (✓) 5. Calibration check completed. Test results 0. 100 AC.
- (✓) 6. Air blank completed.
- (✓) 7. Remove printed record. Attach the record to the completed checklist.

SIGNATURE Sarah Cione

DPS Form Exh G-2 (Rev. 05-01)

INTOXILYZER 8000
Location: TUCSON PD
Serial Number: 80-002201
Core Version: 8105.48
11/08/2013 12:57:58

7 of 7sc
TD4

Standard Lot#: 30412100A1
Last Changed By: R. SZELEWSKI #46927

QAS: S. CIONE #50616
TUCSON PD

Operator: S. CIONE #50616
TUCSON PD

Test	g/210L	Time
Air Blank	0.000	12:58:27
0.100 Cal Check	0.100	12:58:47
Air Blank	0.000	12:59:17

Preventative Maintenance
Performed -- Timer Reset