



CERTIFICATION by CUSTODIAN of RECORDS
Tucson Police Department Crime Laboratory

CU
5.27.08

I hereby certify that these documents are a true and correct copy of the periodic maintenance* for the Intoxilyzer 8000 Serial Number 80-002261 maintained by the Tucson Police Department Crime Laboratory pursuant to the requirements of the Arizona Department of Public Safety for a quality assurance program.

A quality assurance specialist (QAS) tested the instrument on the following dates. The acceptable accuracy limits, as defined in A.A.C. R13-10-104.A.2, for a 0.100AC solution are 0.090AC to 0.110AC.

Date: 5.7.2008 Cal 1 0.101 AC Cal 2 0.101 AC

Between the dates of N/A and N/A the instrument was operating properly and accurately.

The instrument was taken out of service for repair on —
The instrument was returned to service on 5.7.2008

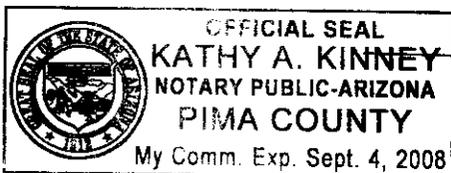
Terry S. Gallegos

Terry S. Gallegos

5.12.2008

ADPS QAS Permit # 33169

SUBSCRIBED AND SWORN to before me this 12, day of May, 2008.



Kathy A Kinney
Notary Public

*Includes documents specified in A.A.C. R13-10-104.A.5

EXHIBIT G-4

THIS REPORT PREPARED PURSUANT TO DUTY IMPOSED BY
A.A.C. R13-10-104(A)

OK
5-27-08
10 of 10
TS4

ARIZONA DEPARTMENT OF PUBLIC SAFETY

STANDARD QUALITY ASSURANCE PROCEDURES
INTOXILYZER MODEL 8000

STANDARD QUALITY ASSURANCE PROCEDURE

QA SPECIALIST Terry Gallegos 20847 AGENCY Tucson Police Department

DATE 5-7-2008 TIME 1338

INTOXILYZER SERIAL # 80-002261 LOCATION Lab

() 1. Display reads "PUSH BUTTON TO START"

DIAGNOSTIC TESTS

- () 1. Clock time check.
- () 2. Date check.

OPERATIONAL TESTS

- () 1. Alcohol-free subject test result 0. 000 AC.
- () 2. Error recognition logic system functioning.
Not a Successfully Completed Test Sequence printed ✓✓✓
- () 3. Proper sample recognition system.
Not a Successfully Completed Test Sequence printed
Deficient sample printed. ✓
- () 4. Standard Calibration Check standard 0. 100 AC
Result: 0. 101 AC

Instrument is operating properly and accurately. YES NO

COMMENTS

SIGNATURE

Terry Gallegos

INTOXILYZER 8000
Location: CMI INC
Serial Number : 80-002261
05/07/2008

13:42:42

OK
2 of 10
TSY

Standard Lot#: 730901I
Last Changed By: T. GALLEGOS #28847

QAS: T. GALLEGOS #28847
TUCSON PD CRIME LAB

Operator: T. GALLEGOS #28847
TUCSON PD CRIME LAB

Subject: SQAP, SQAP
DOB: 11/11/1111
Sex: F Weight: 111

15 Minute Deprivation Period? Yes

Test	g/210L	Time
Air Blank	0.000	13:43:33
Diagnostic Test	Pass	13:44:00
Air Blank	0.000	13:44:28
0.100 Cal Check	0.101	13:44:47
Air Blank	0.000	13:45:16
Subject Test	0.000	13:45:43
Air Blank	0.000	13:46:10
Five Minute Wait	ABT*	
Air Blank	0.000	13:46:45

*Sequence Aborted

Not a Successfully Completed Test Sequence

Pursuant to section 28-1527, Arizona Revised Statutes, this document is a certified duplicate of the information contained in computer storage devices of the Tucson Police Department.

INTOXILYZER 8000
Location: CMI INC
Serial Number : 80-002261
05/07/2008

13:49:47

CM
30 of 10
TS4

Standard Lot#: 730901I
Last Changed By: T. GALLEGOS #28847

QAS: T. GALLEGOS #28847
TUCSON PD CRIME LAB

Operator: T. GALLEGOS #28847
TUCSON PD CRIME LAB

Subject: SQAP, SQAP
DOB: 11/11/1111
Sex: F Weight: 111

15 Minute Deprivation Period? Yes

Test	g/210L	Time
Air Blank	0.000	13:50:38
Diagnostic Test	Pass	13:51:06
Air Blank	IPS*	13:51:20
Air Blank	RFI**	13:51:31

*Improper Sample

**RFI Detect

Not a Successfully Completed Test Sequence

INTOXILYZER 8000
Location: CMI INC
Serial Number : 80-002261
05/07/2008

13:52:06

CM
4 of 10
TS4

Standard Lot#: 730901I
Last Changed By: T. GALLEGOS #28847

QAS: T. GALLEGOS #28847
TUCSON PD CRIME LAB

Operator: T. GALLEGOS #28847
TUCSON PD CRIME LAB

Subject: SQAP, SQAP
DOB: 11/11/1111
Sex: F Weight: 111

15 Minute Deprivation Period? Yes

Test	g/210L	Time
Air Blank	0.000	13:52:58
Diagnostic Test	Pass	13:53:26
Air Blank	0.000	13:53:53
0.100 Cal Check	0.101	13:54:12
Air Blank	0.000	13:54:41
Subject Test	0.064*	13:57:50
Air Blank	0.000	13:58:21
Air Blank	0.000	13:58:48
Subject Test	XXX**	13:59:06
Air Blank	0.000	13:59:40

*Deficient Sample

**Invalid Sample

Begin new deprivation period

Not a Successfully Completed Test Sequence

INTOXILYZER 8000
Location: CMI INC
Serial Number: 80-002261
05/07/2008 14:00:19

OK
50f10
T84

Standard Lot#: 730901I
Last Changed By: T. GALLEGOS #28847

QAS: T. GALLEGOS #28847
TUCSON PD CRIME LAB

Test	g/210L	Time
Air Blank	0.000	14:00:46
Cal Check	0.101	14:01:05
Air Blank	0.000	14:01:35

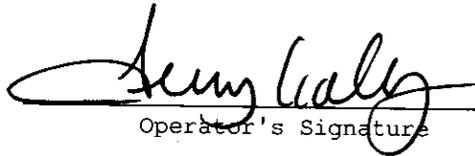

Operator's Signature

EXHIBIT G-2

THIS REPORT PREPARED PURSUANT TO DUTY IMPOSED BY
A.A.C. R13-10-104(A)

ARIZONA DEPARTMENT OF PUBLIC SAFETY

STANDARD QUALITY ASSURANCE PROCEDURES
INTOXILYZER MODEL 8000

STANDARD CALIBRATION CHECK PROCEDURE

OK
5.27-08

60 of 10
154

QA Specialist Terry Gallegos 28847 AGENCY Tucson Police Department
DATE 5.7-2008 TIME 1338
Intoxilyzer Serial # 80-002261 Location Lab

- (✓) 1. Ensure that gas tank is attached to instrument and contains a standard alcohol concentration solution 0. 100 AC.
OR
Pour a standard alcohol concentration solution _____ AC, into a clean dry simulator and assemble the simulator. Ensure that a tight seal has been made. Turn on the simulator and allow temperature to reach 34°C + 0.2°C
- (✓) 2. Intoxilyzer 8000 display reads "PUSH BUTTON TO START"
- (✓) 3. Go to the "Control Testing Menu". Select "D" for dry control test or "W" for wet control test. After selection is made press ENTER.
- (✓) 4. Air blank completed.
- (✓) 5. Calibration check completed. Test results 0. 101 AC.
- (✓) 6. Air blank completed.
- (✓) 7. Remove printed record. Attach the record to the completed checklist.

SIGNATURE Terry Gallegos

DPS Form Exh G-2 (Rev. 05-01)

INTOXILYZER 8000
Location: CMI INC
Serial Number: 80-002261
05/07/2008

13:38:39

Standard Lot#: 730901I
Last Changed By: T. GALLEGOS #28847

QAS: T. GALLEGOS #28847
TUCSON PD CRIME LAB

Test	g/210L	Time
Air Blank	0.000	13:39:07
Cal Check	0.101	13:39:26
Air Blank	0.000	13:39:55

AM
70F10
754



Operator's Signature



TUCSON POLICE DEPARTMENT
CRIME LABORATORY

INTOXILYZER SERVICE RECORD
FOR
CALIBRATION GAS TANK CHANGE

OK 5-27-08

80810
T84

Date: 5.7.2008
 QAS: Terry Gallegos 28847
 Intoxilyzer Serial Number: 80-002261
 New Lot Number: 730901 I
 New Expiration Date: 11.6.2009

- (✓) 1. Intoxilyzer 8000 display reads "PUSH BUTTON TO START"
- (✓) 2. Remove the old gas tank and install the new one.
- (✓) 3. Hit the "ESC" key twice and swipe the QAS card.
- (✓) 4. Go to the "M-Maintenance" menu and select "S-Standard Change." Select "D" for dry gas and enter the following information:
 Enter Target Value: 0.100
 Enter Control Lot #: From the tank label
 Enter Exp Date: From the tank label (mm/dd/yyyy)
 Edit info Y/N? Y or N
 Update Std Info? Y ENTER
 "Please wait saving..."
- (✓) 5. Hit the "ESC" key twice.
- (✓) 6. Go to the "M-Maintenance" menu and select "T-Control Testing." Select "D" for dry control test. After selection is made press ENTER.
- (✓) 7. Air blank completed.
- (✓) 8. Calibration check completed. Test results 0. 102 AC.
- (✓) 9. Air blank completed.
- (✓) 10. Remove and sign printed record. Attach the record to the completed checklist.

SIGNATURE Terry Gallegos

Pursuant to section 28-1327, Arizona Revised Statutes, this document is a certified duplicate of the information contained in computer storage devices of the Tucson Police Department.

INTOXILYZER 8000
Location: CMI INC
Serial Number: 80-002261
05/07/2008

13:35:57

Standard Lot#: 730901I
Last Changed By: 1. 1 #1

QAS: T. GALLEGOS #28847
TUCSON PD CRIME LAB

Test	g/210L	Time
Air Blank	0.000	13:36:25
Cal Check	0.102	13:36:44
Air Blank	0.000	13:37:13

OK
90F10
TS4


Operator's Signature



TUCSON POLICE DEPARTMENT
CRIME LABORATORY

INTOXILYZER SERVICE RECORD

CM
5-27-08
100f10
184

QAS: Terry Gallegos 28847

Intoxilyzer Serial Number: 80-002261

Date Returned to Service: 5.7.2008

CERTIFICATE OF CALIBRATION

INTOXILYZER® 8000

This is to certify that the calibration of INTOXILYZER serial number 70-002261, manufactured by CMI, subsidiary of MPD, Inc. of Owensboro, Kentucky, was tested and found to be in compliance with the National Safety Administration Standard for Devices to Measure Breath Alcohol (F.R., No. 179 48705-48710 Sept. 17, 1993) and with International Recommendation OIML R126 Edition 1998 (E). Calibration solutions are traceable to NIST (NBS) standard material 1828.

Date 4.25.08 Signed 
Technician

EMI INC.

316 EAST 9TH STREET
OWENSBORO, KY. 42303

Pursuant to Section 28.1327, Arizona Revised Statutes, this document is a certified duplicate of the information contained in computer storage devices of the Tucson Police Department.

