



CERTIFICATION by CUSTODIAN of RECORDS
Tucson Police Department Crime Laboratory

154
8-29-08

I hereby certify that these documents are a true and correct copy of the periodic maintenance* for the Intoxilyzer 8000 Serial Number 80-002261 maintained by the Tucson Police Department Crime Laboratory pursuant to the requirements of the Arizona Department of Public Safety for a quality assurance program.

A quality assurance specialist (QAS) tested the instrument on the following dates. The acceptable accuracy limits, as defined in A.A.C. R13-10-104.A.2, for a 0.100AC solution are 0.090AC to 0.110AC.

Date: 8-28-08 Cal 1 0.100 AC Cal 2 0.098 AC

Between the dates of 7-31-08 and 8-28-08 the instrument was operating properly and accurately.

The instrument was taken out of service for repair on N/A.
The instrument was returned to service on N/A.


Clare Conley

Clare L. Conley

8-29-08

ADPS QAS Permit # 33314

SUBSCRIBED AND SWORN to before me this 29th day of August, 2008.

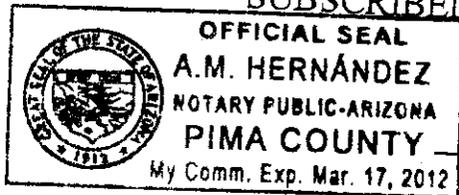

A.M. Hernandez

Notary Public

*Includes documents specified in A.A.C. R13-10-104.A.5

Pursuant to section 28-1327, Arizona Revised Statutes, this document is a certified duplicate of the information contained in computer storage devices of the Tucson Police Department.

EXHIBIT G-4

THIS REPORT PREPARED PURSUANT TO DUTY IMPOSED BY
A.A.C. R13-10-104(A)

ARIZONA DEPARTMENT OF PUBLIC SAFETY
STANDARD QUALITY ASSURANCE PROCEDURES
INTOXILYZER MODEL 8000

STANDARD QUALITY ASSURANCE PROCEDURE

187
cu
TS4
8.29.08

QA SPECIALIST Clare Conley AGENCY Tucson Police Department

DATE 8-28-08 TIME 0827

INTOXILYZER SERIAL # 80-002261 LOCATION ODW DUI HQ

(✓) 1. Display reads "PUSH BUTTON TO START"

DIAGNOSTIC TESTS

(✓) 1. Clock time check.

(✓) 2. Date check.

OPERATIONAL TESTS

(✓) 1. Alcohol-free subject test result 0. 000 AC.

(✓) 2. Error recognition logic system functioning.
Not a Successfully Completed Test Sequence printed

(✓) 3. Proper sample recognition system.
Not a Successfully Completed Test Sequence printed
Deficient sample printed.

(✓) 4. Standard Calibration Check standard 0. 150 AC
Result: 0. 098 AC

Instrument is operating properly and accurately. YES NO

COMMENTS None

SIGNATURE Clare Conley

INTOXILYZER 8000
Location: CMI INC
Serial Number : 80-002261
08/28/2008

08:29:23

2 of 7
cu
104

Standard Lot#: 735401G
Last Changed By: S. CIONE #50616

QAS: C. CONLEY #34517
TUCSON PD

Operator: C. CONLEY #34517
TUCSON PD

Subject: TEST, SQAP

DOB: 11/11/1111

Sex: M

Weight: 111

15 Minute Deprivation Period? Yes

Test	g/210L	Time
Air Blank	0.000	08:30:11
Diagnostic Test	Pass	08:30:38
Air Blank	0.000	08:31:06
0.100 Cal Check	0.100	08:31:24
Air Blank	0.000	08:31:54
Subject Test	0.000	08:32:22
Air Blank	ABT*	08:32:31
Air Blank	0.000	08:32:59

*Sequence Aborted

Not a Successfully Completed Test Sequence

INTOXILYZER 8000
Location: CMI INC
Serial Number : 80-002261
08/28/2008

08:36:21

Standard Lot#: 735401G
Last Changed By: S. CIONE #50616

QAS: C. CONLEY #34517
TUCSON PD

Operator: C. CONLEY #34517
TUCSON PD

Subject: TEST, SQAP
DOB: 11/11/1111
Sex: M Weight: 111

15 Minute Deprivation Period? Yes

Test	g/210L	Time
Air Blank	RFI*	08:37:09
Air Blank	IPS**	08:37:26

*RFI Detect
**Improper Sample

3087
CMI
TS4

Not a Successfully Completed Test Sequence

INTOXILYZER 8000
Location: CMI INC
Serial Number : 80-002261
08/28/2008

08:37:44

Standard Lot#: 735401G
Last Changed By: S. CIONE #50616

QAS: C. CONLEY #34517
TUCSON PD

Operator: C. CONLEY #34517
TUCSON PD

Subject: TEST, SQAP

DOB: 11/11/1111

Sex: M

Weight: 111

15 Minute Deprivation Period? Yes

Test	g/210L	Time
Air Blank	0.000	08:38:34
Diagnostic Test	Pass	08:39:02
Air Blank	0.000	08:39:29
0.100 Cal Check	0.101	08:39:48
Air Blank	0.000	08:40:18
Subject Test	0.397*	08:43:26
Air Blank	0.000	08:43:59
Air Blank	0.000	08:44:26
Subject Test	XXX**	08:44:46
Air Blank	0.000	08:45:20

*Deficient Sample

**Invalid Sample

Begin new deprivation period

Not a Successfully Completed Test Sequence

4567
cu
BY

INTOXILYZER 8000
Location: CMI INC
Serial Number: 80-002261
08/28/2008 08:45:45

5067
CW
124

Standard Lot#: 735401G
Last Changed By: S. CIONE #50616

QAS: C. CONLEY #34517
TUCSON PD

Test	g/210L	Time
Air Blank	0.000	08:46:12
Cal Check	0.098	08:46:31
Air Blank	0.000	08:47:00

Clare Conley

Operator's Signature

EXHIBIT G-2

THIS REPORT PREPARED PURSUANT TO DUTY IMPOSED BY
A.A.C. R13-10-104(A)

ARIZONA DEPARTMENT OF PUBLIC SAFETY
STANDARD QUALITY ASSURANCE PROCEDURES
INTOXILYZER MODEL 8000
STANDARD CALIBRATION CHECK PROCEDURE

687

Cu

TS4
8-29-08

QA Specialist Clare Conley AGENCY Tucson Police Department
DATE 8-28-08 TIME 0827
Intoxilyzer Serial # 80-002261 Location ODW DUI HA

- (✓) 1. Ensure that gas tank is attached to instrument and contains a standard alcohol concentration solution 0. 100 AC.
OR
Pour a standard alcohol concentration solution _____ AC, into a clean dry simulator and assemble the simulator. Ensure that a tight seal has been made. Turn on the simulator and allow temperature to reach 34°C ± 0.2°C
- (✓) 2. Intoxilyzer 8000 display reads "PUSH BUTTON TO START"
- (✓) 3. Go to the "Control Testing Menu". Select "D" for dry control test or "W" for wet control test. After selection is made press ENTER.
- (✓) 4. Air blank completed.
- (✓) 5. Calibration check completed. Test results 0. 100 AC.
- (✓) 6. Air blank completed.
- (✓) 7. Remove printed record. Attach the record to the completed checklist.

SIGNATURE Clare Conley

DPS Form Exh G-2 (Rev. 05-01)

Pursuant to section 28-1327, Arizona Revised Statutes, this document is a certified duplicate of the information contained in computer storage devices of the Tucson Police Department.

INTOXILYZER 8000
Location: CMI INC
Serial Number: 80-002261
08/28/2008

08:27:54

Standard Lot#: 735401G
Last Changed By: S. CIONE #50616

QAS: C. CONLEY #34517
TUCSON PD

Test	g/210L	Time
Air Blank	0.000	08:28:22
Cal Check	0.100	08:28:41
Air Blank	0.000	08:29:10

C. Conley

Operator's Signature

787
cu

104