



EXHIBIT G-4

THIS REPORT PREPARED PURSUANT TO DUTY IMPOSED BY  
A.A.C. R13-10-104(A)

CU  
11-23-07

ARIZONA DEPARTMENT OF PUBLIC SAFETY

STANDARD QUALITY ASSURANCE PROCEDURES  
INTOXILYZER MODEL 8000

1 of 7  
TS4

STANDARD QUALITY ASSURANCE PROCEDURE

QA SPECIALIST Terry Gallegos 20847 AGENCY Tucson Police Department

DATE 10-19-2007 TIME 1445

INTOXILYZER SERIAL # 80-002264 LOCATION DUI HQ (code 12)

( ✓ ) 1. Display reads "PUSH BUTTON TO START"

DIAGNOSTIC TESTS

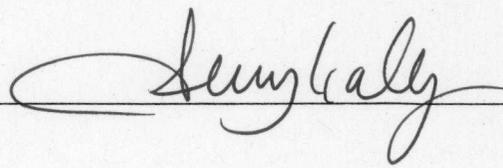
- ( ✓ ) 1. Clock time check.
- ( ✓ ) 2. Date check.

OPERATIONAL TESTS

- ( ✓ ) 1. Alcohol-free subject test result 0. 000 AC.
- ( ✓ ) 2. Error recognition logic system functioning.  
Not a Successfully Completed Test Sequence printed ✓✓✓
- ( ✓ ) 3. Proper sample recognition system.  
Not a Successfully Completed Test Sequence printed  
Deficient sample printed.
- ( ✓ ) 4. Standard Calibration Check standard 0. 100 AC  
Result: 0. 160 AC

Instrument is operating properly and accurately. YES  NO

COMMENTS  
\_\_\_\_\_  
\_\_\_\_\_  
\_\_\_\_\_  
\_\_\_\_\_

SIGNATURE 

Pursuant to section 28-1327, Arizona Revised Statutes, this document is a certified duplicate of the information contained in computer storage devices of the Tucson Police Department.

INTOXILYZER 8000  
Location: TUCSON POLICE DEPT  
Serial Number : 80-002264  
10/19/2007 14:47:06

cu  
2077  
TS4

---

Standard Lot#: 719801I  
Last Changed By: S. SULLIVAN #34971

---

QAS: T. GALLEGOS #28847  
TUCSON PD CRIME LAB

---

Operator: T. GALLEGOS #28847  
TUCSON PD CRIME LAB

---

Subject: SQAP, SQAP  
DOB: 11/11/1111  
Sex: F Weight: 111

---

15 Minute Deprivation Period? Yes

---

Test	g/210L	Time
Air Blank	0.000	14:48:00
Diagnostic Test	Pass	14:48:27
Air Blank	0.000	14:48:55
0.100 Cal Check	0.100	14:49:14
Air Blank	0.000	14:49:43
Subject Test	0.000	14:50:13
Air Blank	0.000	14:50:40
Five Minute Wait	ABT*	
Air Blank	0.000	14:51:14

\*Sequence Aborted

**Not a Successfully Completed Test Sequence**

Pursuant to section 28-1327, Arizona Revised Statutes, this document is a certified duplicate of the information contained in computer storage devices of the Tucson Police Department.

INTOXILYZER 8000  
Location: TUCSON POLICE DEPT  
Serial Number : 80-002264  
10/19/2007

14:51:21

cu  
3 of 7  
TS6

---

Standard Lot#: 719801I  
Last Changed By: S. SULLIVAN #34971

---

QAS: T. GALLEGOS #28847  
TUCSON PD CRIME LAB

---

Operator: T. GALLEGOS #28847  
TUCSON PD CRIME LAB

---

Subject: SQAP, SQAP  
DOB: 11/11/1111  
Sex: F Weight: 111

---

15 Minute Deprivation Period? Yes

---

Test	g/210L	Time
Air Blank	0.000	14:52:05
Diagnostic Test	Pass	14:52:33
Air Blank	0.000	14:53:00
0.100 Cal Check	0.101	14:53:19
Air Blank	RFI*	14:53:25
Air Blank	IPS**	14:53:36

\*RFI Detect

\*\*Improper Sample

### Not a Successfully Completed Test Sequence

Pursuant to section 28-1327, Arizona Revised Statutes, this document is a certified duplicate of the information contained in computer storage devices of the Tucson Police Department.

INTOXILYZER 8000  
Location: TUCSON POLICE DEPT  
Serial Number : 80-002264  
10/19/2007

14:54:12

EM  
4 of 7  
TS4

---

Standard Lot#: 719801I  
Last Changed By: S. SULLIVAN #34971

---

QAS: T. GALLEGOS #28847  
TUCSON PD CRIME LAB

---

Operator: T. GALLEGOS #28847  
TUCSON PD CRIME LAB

---

Subject: SQAP, SQAP  
DOB: 11/11/1111  
Sex: F Weight: 111

---

15 Minute Deprivation Period? Yes

---

Test	g/210L	Time
Air Blank	0.000	14:55:11
Diagnostic Test	Pass	14:55:39
Air Blank	0.000	14:56:06
0.100 Cal Check	0.100	14:56:25
Air Blank	0.000	14:56:54
Subject Test	0.070*	15:00:03
Air Blank	0.000	15:00:34
Air Blank	0.000	15:01:02
Subject Test	XXX**	15:01:20
Air Blank	0.000	15:01:53

\*Deficient Sample

\*\*Invalid Sample

Begin new deprivation period

### Not a Successfully Completed Test Sequence

Pursuant to section 28-1327, Arizona Revised Statutes, this document is a certified duplicate of the information contained in computer storage devices of the Tucson Police Department.

INTOXILYZER 8000

Location: TUCSON POLICE DEPT

Serial Number: 80-002264

10/19/2007

15:02:10

CM  
5 of 7  
TS4

-----  
Standard Lot#: 719801I

Last Changed By: S. SULLIVAN #34971  
-----

QAS: T. GALLEGOS #28847

TUCSON PD CRIME LAB  
-----

Test	g/210L	Time
Air Blank	0.000	15:02:37
Cal Check	0.100	15:02:56
Air Blank	0.000	15:03:26

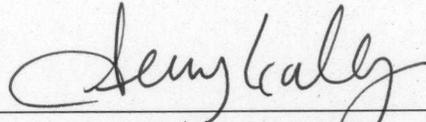
  
-----  
Operator's Signature

EXHIBIT G-2

THIS REPORT PREPARED PURSUANT TO DUTY IMPOSED BY  
A.A.C. R13-10-104(A)

OK  
11-23-07

ARIZONA DEPARTMENT OF PUBLIC SAFETY

STANDARD QUALITY ASSURANCE PROCEDURES  
INTOXILYZER MODEL 8000

6 of 7  
TJ4

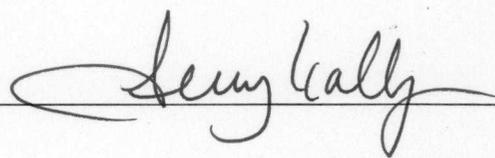
STANDARD CALIBRATION CHECK PROCEDURE

QA Specialist Terry Gallegos 28047 AGENCY Tucson Police Department

DATE 10-19-2007 TIME 1445

Intoxilyzer Serial # 80-002264 Location DUI HQ (code 12)

- ( ✓ ) 1. Ensure that gas tank is attached to instrument and contains a standard alcohol concentration solution 0. 100 AC.  
OR  
Pour a standard alcohol concentration solution \_\_\_\_\_ AC, into a clean dry simulator and assemble the simulator. Ensure that a tight seal has been made. Turn on the simulator and allow temperature to reach 34°C ± 0.2°C
- ( ✓ ) 2. Intoxilyzer 8000 display reads "PUSH BUTTON TO START"
- ( ✓ ) 3. Go to the "Control Testing Menu". Select "D" for dry control test or "W" for wet control test. After selection is made press ENTER.
- ( ✓ ) 4. Air blank completed.
- ( ✓ ) 5. Calibration check completed. Test results 0. 100 AC.
- ( ✓ ) 6. Air blank completed.
- ( ✓ ) 7. Remove printed record. Attach the record to the completed checklist.

SIGNATURE 

DPS Form Exh G-2 (Rev. 05-01)

INTOXILYZER 8000

Location: TUCSON POLICE DEPT

Serial Number: 80-002264

10/19/2007

14:45:27

cu  
7 of 7  
156

-----  
Standard Lot#: 719801I

Last Changed By: S. SULLIVAN #34971  
-----

QAS: T. GALLEGOS #28847

TUCSON PD CRIME LAB  
-----

Test	g/210L	Time
Air Blank	0.000	14:45:55
Cal Check	0.100	14:46:13
Air Blank	0.000	14:46:43

  
Operator's Signature