



CERTIFICATION by CUSTODIAN of RECORDS

Tucson Police Department Crime Laboratory
270 S. Stone Avenue Tucson, AZ 85701-1917

I hereby certify that these documents are a true and correct copy of the periodic maintenance* for the Intoxilyzer 8000 Serial Number 80-002345 maintained by the Tucson Police Department Crime Laboratory pursuant to the requirements of the Arizona Department of Public Safety for a quality assurance program.

134
5.28.09

A quality assurance specialist (QAS) tested the instrument on the following dates. The acceptable accuracy limits, as defined in A.A.C. R13-10-104.A.2, for a 0.100AC solution are 0.090AC to 0.110AC.

Date: 5-28-09 Cal 1 0.102 AC Cal 2 0.102 AC

Between the dates of 5-1-09 and 5-28-09 the instrument was operating properly and accurately.

The instrument was taken out of service for repair on N/A.
The instrument was returned to service on N/A.

Clare Conley

Clare L. Conley


5-28-09

ADPS QAS Permit # 33314

SUBSCRIBED AND SWORN to before me this 28th, day of May, 2009.

A.M. Hernandez

Notary Public

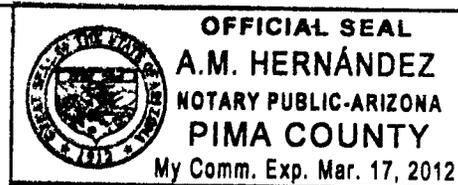

*Includes documents specified in A.A.C. R13-10-104.A.5

THIS REPORT PREPARED PURSUANT TO DUTY IMPOSED BY
A.A.C. R13-10-104(A)

ARIZONA DEPARTMENT OF PUBLIC SAFETY
STANDARD QUALITY ASSURANCE PROCEDURES
INTOXILYZER MODEL 8000
STANDARD QUALITY ASSURANCE PROCEDURE

1587
em
1584
5.28.09

QA SPECIALIST Clare Conley AGENCY Tucson Police Department
DATE 5-28-09 TIME 0823
INTOXILYZER SERIAL # 80-002345 LOCATION ODM

(✓) 1. Display reads "PUSH BUTTON TO START"

DIAGNOSTIC TESTS

- (✓) 1. Clock time check.
- (✓) 2. Date check.

OPERATIONAL TESTS

- (✓) 1. Alcohol-free subject test result 0. 000 AC.
- (✓) 2. Error recognition logic system functioning.
Not a Successfully Completed Test Sequence printed
- (✓) 3. Proper sample recognition system.
Not a Successfully Completed Test Sequence printed
Deficient sample printed.
- (✓) 4. Standard Calibration Check standard 0. 100 AC
Result: 0. 102 AC

Instrument is operating properly and accurately. YES NO

COMMENTS None.

SIGNATURE Clare Conley

INTOXILYZER 8000
Location: ARIZONA
Serial Number : 80-002345
05/28/2009 08:25:07

2067
cu
TS4

Standard Lot#: 826001I
Last Changed By: C. CONLEY #34517

QAS: C. CONLEY #34517
TUCSON PD

Operator: C. CONLEY #34517
TUCSON PD

Subject: TEST,SQAP
DOB: 11/11/1111
Sex: M Weight: 111

15 Minute Deprivation Period? Yes

| Test | g/210L | Time |
|-----------------|--------|----------|
| Air Blank | 0.000 | 08:25:53 |
| Diagnostic Test | Pass | 08:26:20 |
| Air Blank | 0.000 | 08:26:47 |
| 0.100 Cal Check | 0.102 | 08:27:06 |
| Air Blank | 0.000 | 08:27:35 |
| Subject Test | 0.000 | 08:27:55 |
| Air Blank | ABT* | 08:28:03 |
| Air Blank | 0.000 | 08:28:31 |

*Sequence Aborted

Not a Successfully Completed Test Sequence

INTOXILYZER 8000
Location: ARIZONA
Serial Number : 80-002345
05/28/2009 08:28:35

357
u
134

Standard Lot#: 826001I
Last Changed By: C. CONLEY #34517

QAS: C. CONLEY #34517
TUCSON PD

Operator: C. CONLEY #34517
TUCSON PD

Subject: TEST, SQAP
DOB: 11/11/1111
Sex: M Weight: 111

15 Minute Deprivation Period? Yes

| Test | g/210L | Time |
|-----------|--------|----------|
| Air Blank | RFI* | 08:29:02 |
| Air Blank | IPS** | 08:29:14 |

*RFI Detect
**Improper Sample

Not a Successfully Completed Test Sequence

INTOXILYZER 8000
Location: ARIZONA
Serial Number : 80-002345
05/28/2009

08:29:18

Standard Lot#: 826001I
Last Changed By: C. CONLEY #34517

QAS: C. CONLEY #34517
TUCSON PD

Operator: C. CONLEY #34517
TUCSON PD

Subject: TEST,SQAP
DOB: 11/11/1111
Sex: M Weight: 111

15 Minute Deprivation Period? Yes

| Test | g/210L | Time |
|-----------------|--------|----------|
| Air Blank | 0.000 | 08:30:02 |
| Diagnostic Test | Pass | 08:30:30 |
| Air Blank | 0.000 | 08:30:57 |
| 0.100 Cal Check | 0.102 | 08:31:16 |
| Air Blank | 0.000 | 08:31:45 |
| Subject Test | 0.164* | 08:34:53 |
| Air Blank | 0.000 | 08:35:25 |
| Air Blank | 0.000 | 08:35:53 |
| Subject Test | XXX** | 08:36:20 |
| Air Blank | 0.000 | 08:36:54 |

*Deficient Sample

**Invalid Sample

Begin new deprivation period

Not a Successfully Completed Test Sequence

487
C
154

INTOXILYZER 8000

Location: ARIZONA

Serial Number: 80-002345

05/28/2009

08:37:23

Standard Lot#: 826001I

Last Changed By: C. CONLEY #34517

QAS: C. CONLEY #34517

TUCSON PD

| Test | g/210L | Time |
|-----------|--------|----------|
| Air Blank | 0.000 | 08:37:51 |
| Cal Check | 0.102 | 08:38:10 |
| Air Blank | 0.000 | 08:38:39 |

C. Conley

Operator's Signature

557
C
104

EXHIBIT G-2

THIS REPORT PREPARED PURSUANT TO DUTY IMPOSED BY
A.A.C. R13-10-104(A)

ARIZONA DEPARTMENT OF PUBLIC SAFETY

STANDARD QUALITY ASSURANCE PROCEDURES
INTOXILYZER MODEL 8000

STANDARD CALIBRATION CHECK PROCEDURE

6 of 7
cu
By
5-28-09

QA Specialist Clare Conley AGENCY Tucson Police Department
DATE 5-28-09 TIME 0823
Intoxilyzer Serial # 80-002345 Location ODM

- (✓) 1. Ensure that gas tank is attached to instrument and contains a standard alcohol concentration solution 0. 100 AC.
OR
Pour a standard alcohol concentration solution _____ AC, into a clean dry simulator and assemble the simulator. Ensure that a tight seal has been made. Turn on the simulator and allow temperature to reach 34°C ± 0.2°C
- (✓) 2. Intoxilyzer 8000 display reads "PUSH BUTTON TO START"
- (✓) 3. Go to the "Control Testing Menu". Select "D" for dry control test or "W" for wet control test. After selection is made press ENTER.
- (✓) 4. Air blank completed.
- (✓) 5. Calibration check completed. Test results 0. 102 AC.
- (✓) 6. Air blank completed.
- (✓) 7. Remove printed record. Attach the record to the completed checklist.

SIGNATURE Clare Conley

DPS Form Exh G-2 (Rev. 05-01)

INTOXILYZER 8000

Location: ARIZONA

Serial Number: 80-002345

05/28/2009

08:23:45

Standard Lot#: 826001I

Last Changed By: C. CONLEY #34517

QAS: C. CONLEY #34517

TUCSON PD

| Test | g/210L | Time |
|-----------|--------|----------|
| Air Blank | 0.000 | 08:24:12 |
| Cal Check | 0.102 | 08:24:31 |
| Air Blank | 0.000 | 08:25:00 |

Clare Conley

Operator's Signature

787
cu
BY