



CERTIFICATION by CUSTODIAN of RECORDS

Tucson Police Department Crime Laboratory
270 S. Stone Avenue Tucson, AZ 85701-1917

By
8-3-2010

I hereby certify that these documents are a true and correct copy of the periodic maintenance* for the Intoxilyzer 8000 Serial Number 80-002345 maintained by the Tucson Police Department Crime Laboratory pursuant to the requirements of the Arizona Department of Public Safety for a quality assurance program.

A quality assurance specialist (QAS) tested the instrument on the following dates. The acceptable accuracy limits, as defined in A.A.C. R13-10-104.A.2, for a 0.100AC solution are 0.090AC to 0.110AC.

Date: 07/29/10 Cal 1 0.101 AC Cal 2 0.110 AC

Between the dates of 07/01/10 and 07/29/10 the instrument was operating properly and accurately.

The instrument was taken out of service for repair on N/A.
The instrument was returned to service on N/A.

Cheryl K. Straub

Cheryl K. Straub


08/02/10

ADPS QAS Permit # 33408

SUBSCRIBED AND SWORN to before me this 2, day of August, 2010.

A.M. Hernandez

Notary Public

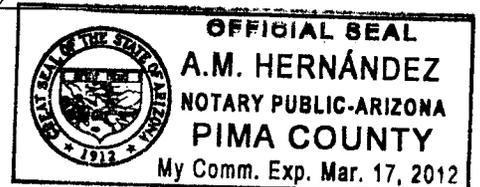

*Includes documents specified in A.A.C. R13-10-104.A.5

127
CS

THIS REPORT PREPARED PURSUANT TO DUTY IMPOSED BY
A.A.C. R13-10-104(A)

ARIZONA DEPARTMENT OF PUBLIC SAFETY
STANDARD QUALITY ASSURANCE PROCEDURES
INTOXILYZER MODEL 8000
STANDARD QUALITY ASSURANCE PROCEDURE

TSY
8.3.2010

QA SPECIALIST Cheryl STRAUB AGENCY Tucson Police Department

DATE 07/29/10 TIME 6:44

INTOXILYZER SERIAL # B0-002345 LOCATION TEAM 3

(✓) 1. Display reads "PUSH BUTTON TO START"

DIAGNOSTIC TESTS

- (✓) 1. Clock time check.
- (✓) 2. Date check.

OPERATIONAL TESTS

- (✓) 1. Alcohol-free subject test result 0. 000 AC.
- (✓) 2. Error recognition logic system functioning.
Not a Successfully Completed Test Sequence printed
- (✓) 3. Proper sample recognition system.
Not a Successfully Completed Test Sequence printed
Deficient sample printed.
- (✓) 4. Standard Calibration Check standard 0. 100 AC
Result: 0. 100 AC

Instrument is operating properly and accurately. YES NO

COMMENTS

SIGNATURE Cheryl Straub

Pursuant to section 28-1327, Arizona Revised Statutes, this document is a certified duplicate of the information contained in computer storage devices of the Tucson Police Department.

277
CS

INTOXILYZER 8000
Location: ARIZONA
Serial Number : 80-002345
07/29/2010

06:46:22

TSh

Standard Lot#: 642845
Last Changed By: C. STRAUB #50772

QAS: C. STRAUB #50772
TUCSON PD

Operator: C. STRAUB #50772
TUCSON PD

Subject: SQAP, SQAP
DOB: 11/11/1111
Sex: F Weight: 111

15 Minute Deprivation Period? Yes

| Test | g/210L | Time |
|-----------------|--------|----------|
| Air Blank | 0.000 | 06:47:19 |
| Diagnostic Test | Pass | 06:47:46 |
| Air Blank | 0.000 | 06:48:14 |
| 0.100 Cal Check | 0.101 | 06:48:32 |
| Air Blank | 0.000 | 06:49:02 |
| Subject Test | 0.000 | 06:49:44 |
| Air Blank | ABT* | 06:49:50 |
| Air Blank | 0.000 | 06:50:19 |

*Sequence Aborted

Not a Successfully Completed Test Sequence

387
CS

INTOXILYZER 8000
Location: ARIZONA
Serial Number : 80-002345
07/29/2010

06:50:22

134

Standard Lot#: 642845
Last Changed By: C. STRAUB #50772

QAS: C. STRAUB #50772
TUCSON PD

Operator: C. STRAUB #50772
TUCSON PD

Subject: SQAP, SQAP
DOB: 11/11/1111
Sex: F Weight: 111

15 Minute Deprivation Period? Yes

| Test | g/210L | Time |
|-----------|--------|----------|
| Air Blank | RFI* | 06:50:53 |
| Air Blank | IPS** | 06:51:01 |

*RFI Detect
**Improper Sample

Not a Successfully Completed Test Sequence

487
CS

184

INTOXILYZER 8000
Location: ARIZONA
Serial Number : 80-002345
07/29/2010

06:51:06

Standard Lot#: 642845
Last Changed By: C. STRAUB #50772

QAS: C. STRAUB #50772
TUCSON PD

Operator: C. STRAUB #50772
TUCSON PD

Subject: SQAP, SQAP
DOB: 11/11/1111
Sex: F Weight: 111

15 Minute Deprivation Period? Yes

| Test | g/210L | Time |
|-----------------|--------|----------|
| Air Blank | 0.000 | 06:51:58 |
| Diagnostic Test | Pass | 06:52:25 |
| Air Blank | 0.000 | 06:52:53 |
| 0.100 Cal Check | 0.101 | 06:53:11 |
| Air Blank | 0.000 | 06:53:41 |
| Subject Test | 0.098* | 06:56:49 |
| Air Blank | 0.000 | 06:57:22 |
| Air Blank | 0.000 | 06:57:49 |
| Subject Test | XXX** | 06:58:12 |
| Air Blank | 0.000 | 06:58:47 |

*Deficient Sample

**Invalid Sample

Begin new deprivation period

Not a Successfully Completed Test Sequence

57
CS


INTOXILYZER 8000
Location: ARIZONA
Serial Number: 80-002345
07/29/2010 06:59:07

104

Standard Lot#: 642845
Last Changed By: C. STRAUB #50772

QAS: C. STRAUB #50772
TUCSON PD

| Test | g/210L | Time |
|-----------|--------|----------|
| Air Blank | 0.000 | 06:59:34 |
| Cal Check | 0.100 | 06:59:53 |
| Air Blank | 0.000 | 07:00:22 |

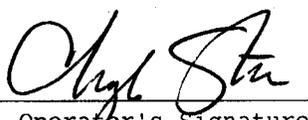

Operator's Signature

677
CS

THIS REPORT PREPARED PURSUANT TO DUTY IMPOSED BY
A.A.C. R13-10-104(A)

ARIZONA DEPARTMENT OF PUBLIC SAFETY

STANDARD QUALITY ASSURANCE PROCEDURES
INTOXILYZER MODEL 8000

STANDARD CALIBRATION CHECK PROCEDURE

BSY
8.3.2010

QA Specialist Cheryl STRAUB AGENCY Tucson Police Department
DATE 07/29/10 TIME 6:44
Intoxilyzer Serial # 80-002345 Location TEAM 3

- (✓) 1. Ensure that gas tank is attached to instrument and contains a standard alcohol concentration solution 0. 100 AC.
OR
Pour a standard alcohol concentration solution N/A AC, into a clean dry simulator and assemble the simulator. Ensure that a tight seal has been made. Turn on the simulator and allow temperature to reach 34°C ± 0.2°C
- (✓) 2. Intoxilyzer 8000 display reads "PUSH BUTTON TO START"
- (✓) 3. Go to the "Control Testing Menu". Select "D" for dry control test or "W" for wet control test. After selection is made press ENTER.
- (✓) 4. Air blank completed.
- (✓) 5. Calibration check completed. Test results 0. 101 AC.
- (✓) 6. Air blank completed.
- (✓) 7. Remove printed record. Attach the record to the completed checklist.

SIGNATURE Cheryl Straub

Pursuant to section 28-1327, Arizona Revised Statutes, this document is a certified duplicate of the information contained in computer storage devices of the Tucson Police Department.

787
CS

BS4

INTOXILYZER 8000
Location: ARIZONA
Serial Number: 80-002345
07/29/2010 06:44:58

Standard Lot#: 642845
Last Changed By: C. STRAUB #50772

QAS: C. STRAUB #50772
TUCSON PD

| Test | g/210L | Time |
|-----------|--------|----------|
| Air Blank | 0.000 | 06:45:25 |
| Cal Check | 0.101 | 06:45:44 |
| Air Blank | 0.000 | 06:46:13 |



Operator's Signature