



CERTIFICATION by CUSTODIAN of RECORDS

Tucson Police Department Crime Laboratory
270 S. Stone Avenue Tucson, AZ 85701-1917

TS4
2-10-2011

I hereby certify that these documents are a true and correct copy of the periodic maintenance* for the Intoxilyzer 8000 Serial Number 80-002345 maintained by the Tucson Police Department Crime Laboratory pursuant to the requirements of the Arizona Department of Public Safety for a quality assurance program.

A quality assurance specialist (QAS) tested the instrument on the following dates. The acceptable accuracy limits, as defined in A.A.C. R13-10-104.A.2, for a 0.100AC solution are 0.090AC to 0.110AC.

Date: 1/10/2011 Cal 1 N/A AC Cal 2 N/A AC

Between the dates of - and - the instrument was operating properly and accurately.

The instrument was taken out of service for repair on 1/10/2011.
The instrument was returned to service on -.

Sarah Cione

Sarah L. Cione


2/10/11

ADPS QAS Permit # 33355

SUBSCRIBED AND SWORN to before me this 10, day of February, 2011.

A.M. Hernandez

Notary Public

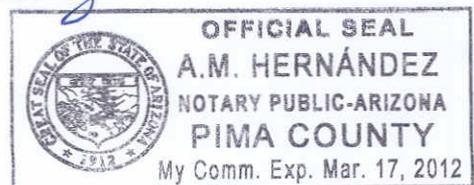

*Includes documents specified in A.A.C. R13-10-104.A.5



TUCSON POLICE DEPARTMENT
CRIME LABORATORY

1 of 1 SC

INTOXILYZER SERVICE RECORD

TSD
2-10-2011

Date: 1/10/2011

QAS: Sarah Cione

Intoxilyzer Serial Number: 80-002345

Reason For Service: Diagnostic Failure - temperature regulation.
Crime Lab notified by Officers Cnos that intox was not
working.

Date Out of Service: 1/10/2011

Calibration Check completed prior to removal from service

Date: N/A

Not able to complete calibration check
or SQAP because instrument does not
pass Diagnostics, & will not go to
ready mode.

SQAP completed prior to removal from service

Date: N/A

Corrective Action: Sent to CMI, Inc.

In lab for troubleshooting