



CERTIFICATION by CUSTODIAN of RECORDS

Tucson Police Department Crime Laboratory
270 S. Stone Avenue Tucson, AZ 85701-1917

CM
3-16-11

I hereby certify that these documents are a true and correct copy of the periodic maintenance* for the Intoxilyzer 8000 Serial Number 80-002345 maintained by the Tucson Police Department Crime Laboratory pursuant to the requirements of the Arizona Department of Public Safety for a quality assurance program.

A quality assurance specialist (QAS) tested the instrument on the following dates. The acceptable accuracy limits, as defined in A.A.C. R13-10-104.A.2, for a 0.100AC solution are 0.090AC to 0.110AC.

Date: 03/09/2011 Cal 1 0.101 AC Cal 2 0.101 AC

Between the dates of 02/09/2011 and 03/09/2011 the instrument was operating properly and accurately.

The instrument was taken out of service for repair on N/A.
The instrument was returned to service on N/A.

Cheryl K. Straub

Cheryl K. Straub


03/16/2011

ADPS QAS Permit # 33408

SUBSCRIBED AND SWORN to before me this 16, day of March, 20 11.

A.M. Hernandez

Notary Public

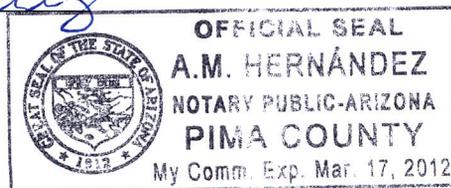

*Includes documents specified in A.A.C. R13-10-104.A.5

197 CS

THIS REPORT PREPARED PURSUANT TO DUTY IMPOSED BY
A.A.C. R13-10-104(A)

ARIZONA DEPARTMENT OF PUBLIC SAFETY

STANDARD QUALITY ASSURANCE PROCEDURES
INTOXILYZER MODEL 8000

STANDARD QUALITY ASSURANCE PROCEDURE

Ch
3-16-11

QA SPECIALIST Cheryl STRAUB AGENCY Tucson Police Department

DATE 03/09/2011 TIME 14:08

INTOXILYZER SERIAL # 80-002345 LOCATION CRIME LAB

(✓) 1. Display reads "PUSH BUTTON TO START"

DIAGNOSTIC TESTS

- (✓) 1. Clock time check.
- (✓) 2. Date check.

OPERATIONAL TESTS

- (✓) 1. Alcohol-free subject test result 0. 000 AC.
- (✓) 2. Error recognition logic system functioning.
Not a Successfully Completed Test Sequence printed
- (✓) 3. Proper sample recognition system.
Not a Successfully Completed Test Sequence printed
Deficient sample printed.
- (✓) 4. Standard Calibration Check standard 0. 100 AC
Result: 0. 101 AC

Instrument is operating properly and accurately. YES NO

COMMENTS

SIGNATURE Cheryl Straub

Pursuant to section 28-1327, Arizona Revised Statutes, this document is a certified duplicate of the information contained in computer storage devices of the Tucson Police Department.

277
CS

INTOXILYZER 8000
Location: ARIZONA
Serial Number : 80-002345
03/09/2011 14:13:30

ln

Standard Lot#: 20910100A1
Last Changed By: C. STRAUB #50772

QAS: C. STRAUB #50772
TUCSON PD

Operator: C. STRAUB #50772
TUCSON PD

Subject: SQAP, SQAP
DOB: 11/11/1111
Sex: F Weight: 111

15 Minute Deprivation Period? Yes

Test	g/210L	Time
Air Blank	0.000	14:14:41
Diagnostic Test	Pass	14:15:09
Air Blank	0.000	14:15:36
0.100 Cal Check	0.102	14:15:55
Air Blank	0.000	14:16:24
Subject Test	0.000	14:16:38
Air Blank	ABT*	14:16:44
Air Blank	0.000	14:17:12

*Sequence Aborted

Not a Successfully Completed Test Sequence

Pursuant to section 28-1327, Arizona Revised Statutes, this document is a certified duplicate of the information contained in computer storage devices of the Tucson Police Department.

317
C8

INTOXILYZER 8000
Location: ARIZONA
Serial Number : 80-002345
03/09/2011 14:17:20

Ch

Standard Lot#: 20910100A1 °
Last Changed By: C. STRAUB #50772

QAS: C. STRAUB #50772
TUCSON PD

Operator: C. STRAUB #50772
TUCSON PD

Subject: SQAP, SQAP
DOB: 11/11/1111
Sex: F Weight: 111

15 Minute Deprivation Period? Yes

Test	g/210L	Time
Air Blank	RFI*	14:18:27
Air Blank	IPS**	14:18:35

*RFI Detect
**Improper Sample

Not a Successfully Completed Test Sequence

Pursuant to section 28-1327, Arizona Revised Statutes, this document is a certified duplicate of the information contained in computer storage devices of the Tucson Police Department.

497
C8

INTOXILYZER 8000
Location: ARIZONA
Serial Number : 80-002345
03/09/2011

14:18:46

Ch

Standard Lot#: 20910100A1
Last Changed By: C. STRAUB #50772

QAS: C. STRAUB #50772
TUCSON PD

Operator: C. STRAUB #50772
TUCSON PD

Subject: SQAP, SQAP
DOB: 11/11/1111
Sex: F Weight: 111

15 Minute Deprivation Period? Yes

Test	g/210L	Time
Air Blank	0.000	14:20:07
Diagnostic Test	Pass	14:20:34
Air Blank	0.000	14:21:02
0.100 Cal Check	0.102	14:21:21
Air Blank	0.000	14:21:50
Subject Test	0.250*	14:24:58
Air Blank	0.000	14:25:31
Air Blank	0.000	14:25:58
Subject Test	XXX**	14:26:24
Air Blank	0.000	14:26:58

*Deficient Sample

**Invalid Sample

Begin new deprivation period

Not a Successfully Completed Test Sequence

Pursuant to section 28-1327, Arizona Revised Statutes, this document is a certified duplicate of the information contained in computer storage devices of the Tucson Police Department.

577
CS

INTOXILYZER 8000
Location: ARIZONA
Serial Number: 80-002345
03/09/2011 14:27:39

CS

Standard Lot#: 20910100A1
Last Changed By: C. STRAUB #50772

QAS: C. STRAUB #50772
TUCSON PD

Test	g/210L	Time
Air Blank	0.000	14:28:07
Cal Check	0.101	14:28:25
Air Blank	0.000	14:28:55



Operator's Signature

EXHIBIT G-2

677
CS

THIS REPORT PREPARED PURSUANT TO DUTY IMPOSED BY
A.A.C. R13-10-104(A)

ARIZONA DEPARTMENT OF PUBLIC SAFETY

STANDARD QUALITY ASSURANCE PROCEDURES
INTOXILYZER MODEL 8000

STANDARD CALIBRATION CHECK PROCEDURE

CU
3-16-11

QA Specialist Cheryl STRAUB AGENCY Tucson Police Department
DATE 03/09/2011 TIME 14:08
Intoxilyzer Serial # 80-002345 Location CRIME LAB

- (✓) 1. Ensure that gas tank is attached to instrument and contains a standard alcohol concentration solution 0. 100 AC.
OR
Pour a standard alcohol concentration solution N/A AC, into a clean dry simulator and assemble the simulator. Ensure that a tight seal has been made. Turn on the simulator and allow temperature to reach 34°C ± 0.2°C
- (✓) 2. Intoxilyzer 8000 display reads "PUSH BUTTON TO START"
- (✓) 3. Go to the "Control Testing Menu". Select "D" for dry control test or "W" for wet control test. After selection is made press ENTER.
- (✓) 4. Air blank completed.
- (✓) 5. Calibration check completed. Test results 0. 101 AC.
- (✓) 6. Air blank completed.
- (✓) 7. Remove printed record. Attach the record to the completed checklist.

SIGNATURE Cheryl Straub

DPS Form Exh G-2 (Rev. 05-01)

777
CS

INTOXILYZER 8000
Location: ARIZONA
Serial Number: 80-002345
03/09/2011 14:08:48

Standard Lot#: 20910100A1
Last Changed By: C. STRAUB #50772

CS

QAS: C. STRAUB #50772
TUCSON PD

Test	g/210L	Time
Air Blank	0.000	14:09:16
Cal Check	0.101	14:09:34
Air Blank	0.000	14:10:04



Operator's Signature