



CERTIFICATION by CUSTODIAN of RECORDS  
 Tucson Police Department Crime Laboratory  
 1306 W. Miracle Mile, Tucson, AZ 85705

I hereby certify that these documents are a true and correct copy of the periodic maintenance\* for the Intoxilyzer 8000 Serial Number 80-002345 maintained by the Tucson Police Department Crime Laboratory pursuant to the requirements of the Arizona Department of Public Safety for a quality assurance program.

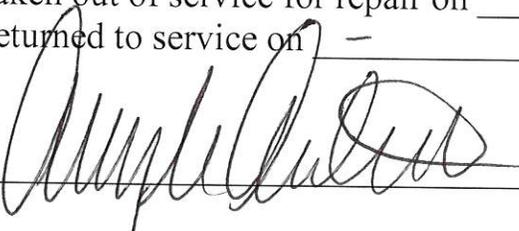
TS4  
6-1-2015

A quality assurance specialist (QAS) tested the instrument on the following dates. The acceptable accuracy limits, as defined in A.A.C. R13-10-104.A.2, for a 0.100AC solution are 0.090AC to 0.110AC.

Date: 5-29-15 Cal 1 0.101 AC Cal 2 0.100 AC

Between the dates of 5-1-15 and 5-29-15 the instrument was operating properly and accurately.

The instrument was taken out of service for repair on \_\_\_\_\_.  
 The instrument was returned to service on \_\_\_\_\_.

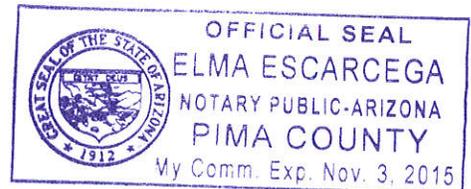
  
 \_\_\_\_\_  
 Amy L. Autret  
6-1-15

ADPS QAS Permit # 33718

SUBSCRIBED AND SWORN to before me this 18<sup>th</sup> day of June, 2015.

  
 \_\_\_\_\_

Notary Public



\*Includes documents specified in A.A.C. R13-10-104.A.5

EXHIBIT G-4

THIS REPORT PREPARED PURSUANT TO DUTY IMPOSED BY  
A.A.C. R13-10-104(A)

1 of 7  
JLS  
TSY  
6.1.2015

ARIZONA DEPARTMENT OF PUBLIC SAFETY

STANDARD QUALITY ASSURANCE PROCEDURES  
INTOXILYZER MODEL 8000

STANDARD QUALITY ASSURANCE PROCEDURE

QA SPECIALIST Amy Autret 53546 AGENCY Tucson Police Department

DATE 5-29-15 TIME 1140

INTOXILYZER SERIAL # 80-002345 LOCATION 000

(✓) 1. Display reads "PUSH BUTTON TO START"

DIAGNOSTIC TESTS

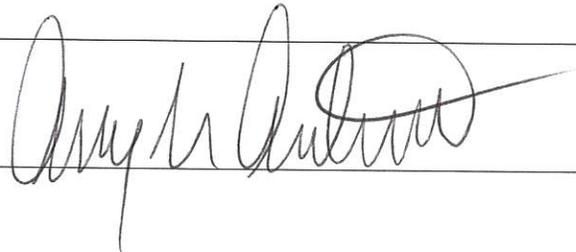
- (✓) 1. Clock time check.
- (✓) 2. Date check.

OPERATIONAL TESTS

- (✓) 1. Alcohol-free subject test result 0. 000 AC.
- (✓) 2. Error recognition logic system functioning.  
Not a Successfully Completed Test Sequence printed
- (✓) 3. Proper sample recognition system.  
Not a Successfully Completed Test Sequence printed  
Deficient sample printed.
- (✓) 4. Standard Calibration Check standard 0. 100 AC  
Result: 0. 100 AC

Instrument is operating properly and accurately. YES  NO

COMMENTS  
\_\_\_\_\_  
\_\_\_\_\_  
\_\_\_\_\_  
\_\_\_\_\_

SIGNATURE 

Pursuant to section 28-1327, Arizona Revised Statutes, this document is a certified duplicate of the information contained in computer storage devices of the Tucson Police Department.

INTOXILYZER 8000  
Location:  
Serial Number: 80-002345  
Core Version: 8105.48  
05/29/2015

11:42:14

2 of 7  
MA  
TS4

---

Standard Lot#: 25414100A4  
Last Changed By: A. AUTRET #53546

---

QAS: A. AUTRET #53546  
TUCSON PD

---

Operator: A. AUTRET #53546  
TUCSON PD

---

Subject: SQAP, SQAP  
DOB: 11/11/1987  
Sex: F Weight: 111

---

15 Minute Deprivation Period? Yes

---

Test	g/210L	Time
Air Blank	0.000	11:43:08
Diagnostic Test	Pass	11:43:43
Air Blank	0.000	11:44:10
0.100 Cal Check	0.100	11:44:31
Air Blank	0.000	11:45:00
Subject Test	0.000	11:45:17
Air Blank	0.000	11:45:44
Wait	ABT*	
Air Blank	0.000	11:46:19

\*Sequence Aborted

### Not a Successfully Completed Test Sequence

Pursuant to section 28-1327, Arizona Revised Statutes, this document is a certified duplicate of the information contained in computer storage devices of the Tucson Police Department.

INTOXILYZER 8000  
Location:  
Serial Number: 80-002345  
Core Version: 8105.48  
05/29/2015

11:46:37

3 of 7  
AA  
TS4

---

Standard Lot#: 25414100A4  
Last Changed By: A. AUTRET #53546

---

QAS: A. AUTRET #53546  
TUCSON PD

---

Operator: A. AUTRET #53546  
TUCSON PD

---

Subject: SQAP, SQAP  
DOB: 11/11/1987  
Sex: F Weight: 111

---

15 Minute Deprivation Period? Yes

---

Test	g/210L	Time
Air Blank	0.000	11:47:32
Diagnostic Test	Pass	11:48:07
Air Blank	0.000	11:48:35
0.100 Cal Check	RFI*	11:48:49
Air Blank	IPS**	11:48:57

\*RFI Detect  
\*\*Improper Sample

### Not a Successfully Completed Test Sequence

Pursuant to section 28-1327, Arizona Revised Statutes, this document is a certified duplicate of the information contained in computer storage devices of the Tucson Police Department.

INTOXILYZER 8000  
Location:  
Serial Number: 80-002345  
Core Version: 8105.48  
05/29/2015 11:49:17

4 of 7  
JL  
B4

---

Standard Lot#: 25414100A4  
Last Changed By: A. AUTRET #53546

---

QAS: A. AUTRET #53546  
TUCSON PD

---

Operator: A. AUTRET #53546  
TUCSON PD

---

Subject: SQAP, SQAP  
DOB: 11/11/1987  
Sex: F Weight: 111

---

15 Minute Deprivation Period? Yes

---

Test	g/210L	Time
Air Blank	0.000	11:50:19
Diagnostic Test	Pass	11:50:54
Air Blank	0.000	11:51:21
0.100 Cal Check	0.100	11:51:42
Air Blank	0.000	11:52:12
Subject Test	0.155*	11:55:19
Air Blank	0.000	11:55:51
Air Blank	0.000	11:56:18
Subject Test	XXX**	11:56:47
Air Blank	0.000	11:57:21

\*Deficient Sample  
\*\*Invalid Sample  
Begin new deprivation period

**Not a Successfully Completed Test Sequence**

Pursuant to section 28-1327, Arizona Revised Statutes, this document is a certified duplicate of the information contained in computer storage devices of the Tucson Police Department.

INTOXILYZER 8000  
Location:  
Serial Number: 80-002345  
Core Version: 8105.48  
05/29/2015 11:57:51

5 of 7  
add  
TB4

-----  
Standard Lot#: 25414100A4  
Last Changed By: A. AUTRET #53546  
-----

QAS: A. AUTRET #53546  
TUCSON PD  
-----

Operator: A. AUTRET #53546  
TUCSON PD  
-----

Test	g/210L	Time
Air Blank	0.000	11:58:20
0.100 Cal Check	0.100	11:58:41
Air Blank	0.000	11:59:11

Preventative Maintenance  
Performed -- Timer Reset

EXHIBIT G-2

THIS REPORT PREPARED PURSUANT TO DUTY IMPOSED BY  
A.A.C. R13-10-104(A)

ARIZONA DEPARTMENT OF PUBLIC SAFETY

STANDARD QUALITY ASSURANCE PROCEDURES  
INTOXILYZER MODEL 8000

STANDARD CALIBRATION CHECK PROCEDURE

6 of 7  
JLB  
TSH  
6-1-2015

QA Specialist Amy Autret 53546 AGENCY Tucson Police Department

DATE 5-29-15 TIME 1140

Intoxilyzer Serial # 80-002345 Location OPD

- (✓) 1. Ensure that gas tank is attached to instrument and contains a standard alcohol concentration solution 0. 100 AC.  
OR  
Pour a standard alcohol concentration solution \_\_\_\_\_ AC, into a clean dry simulator and assemble the simulator. Ensure that a tight seal has been made. Turn on the simulator and allow temperature to reach 34°C ± 0.2°C
- (✓) 2. Intoxilyzer 8000 display reads "PUSH BUTTON TO START"
- (✓) 3. Go to the "Control Testing Menu". Select "D" for dry control test or "W" for wet control test. After selection is made press ENTER.
- (✓) 4. Air blank completed.
- (✓) 5. Calibration check completed. Test results 0. 101 AC.
- (✓) 6. Air blank completed.
- (✓) 7. Remove printed record. Attach the record to the completed checklist.

SIGNATURE \_\_\_\_\_



DPS Form Exh G-2 (Rev. 05-01)

INTOXILYZER 8000  
Location:  
Serial Number: 80-002345  
Core Version: 8105.48  
05/29/2015 11:40:02

7 of 7  
MB

TS4

-----  
Standard Lot#: 25414100A4  
Last Changed By: A. AUTRET #53546  
-----

QAS: A. AUTRET #53546  
TUCSON PD  
-----

Operator: A. AUTRET #53546  
TUCSON PD  
-----

Test	g/210L	Time
Air Blank	0.000	11:40:31
0.100 Cal Check	0.101	11:40:52
Air Blank	0.000	11:41:22

Preventative Maintenance  
Performed -- Timer Reset