



CERTIFICATION by CUSTODIAN of RECORDS  
 Tucson Police Department Crime Laboratory  
 1306 W. Miracle Mile, Tucson, AZ 85705

TSK  
 12-18-2015

I hereby certify that these documents are a true and correct copy of the periodic maintenance\* for the Intoxilyzer 8000 Serial Number 80-002345 maintained by the Tucson Police Department Crime Laboratory pursuant to the requirements of the Arizona Department of Public Safety for a quality assurance program.

A quality assurance specialist (QAS) tested the instrument on the following dates. The acceptable accuracy limits, as defined in A.A.C. R13-10-104.A.2, for a 0.100AC solution are 0.090AC to 0.110AC.

Date: 12-11-15 Cal 1 0.101 AC Cal 2 0.100 AC

Between the dates of 11-13-15 and 12-11-15 the instrument was operating properly and accurately.

The instrument was taken out of service for repair on \_\_\_\_\_.  
 The instrument was returned to service on \_\_\_\_\_.

*[Handwritten Signature]*

Amy L. Autret


12-16-15

ADPS QAS Permit # 33718

SUBSCRIBED AND SWORN to before me this 16, day of December, 20 15.

*[Handwritten Signature]*

Notary Public

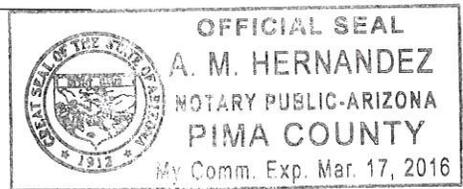

\*Includes documents specified in A.A.C. R13-10-104.A.5

EXHIBIT G-4

THIS REPORT PREPARED PURSUANT TO DUTY IMPOSED BY  
A.A.C. R13-10-104(A)

ARIZONA DEPARTMENT OF PUBLIC SAFETY  
STANDARD QUALITY ASSURANCE PROCEDURES  
INTOXILYZER MODEL 8000

STANDARD QUALITY ASSURANCE PROCEDURE

10FB  
JLA  
TSY  
12-18-2015

QA SPECIALIST Amy Autry 53546 AGENCY Tucson Police Department

DATE 12-11-15 TIME 1123

INTOXILYZER SERIAL # 80-002345 LOCATION 000

( ✓ ) 1. Display reads "PUSH BUTTON TO START"

DIAGNOSTIC TESTS

- ( ✓ ) 1. Clock time check.
- ( ✓ ) 2. Date check.

OPERATIONAL TESTS

- ( ✓ ) 1. Alcohol-free subject test result 0. 000 AC.
- ( ✓ ) 2. Error recognition logic system functioning.  
Not a Successfully Completed Test Sequence printed
- ( ✓ ) 3. Proper sample recognition system.  
Not a Successfully Completed Test Sequence printed  
Deficient sample printed.
- ( ✓ ) 4. Standard Calibration Check standard 0. 100 AC  
Result: 0. 100 AC

Instrument is operating properly and accurately. YES  NO

COMMENTS \_\_\_\_\_  
\_\_\_\_\_  
\_\_\_\_\_

SIGNATURE 

INTOXILYZER 8000

Location:

Serial Number: 80-002345

Core Version: 8105.48

12/11/2015

11:25:22

*2018  
JW  
754*

---

Standard Lot#: 25414100A4

Last Changed By: A. AUTRET #53546

---

QAS: A. AUTRET #53546

TUCSON PD

---

Operator: A. AUTRET #53546

TUCSON PD

---

Subject: SQAP, SQAP

DOB: 11/11/1987

Sex: F Weight: 111

---

15 Minute Deprivation Period? Yes

---

Test	g/210L	Time
Air Blank	0.000	11:27:05
Diagnostic Test	Pass	11:27:40
Air Blank	0.000	11:28:08
0.100 Cal Check	0.101	11:28:28
Air Blank	0.000	11:28:58
Subject Test	0.000	11:29:20
Air Blank	0.000	11:29:47
Wait	ABT*	
Air Blank	0.000	11:30:22

\*Sequence Aborted

**Not a Successfully Completed Test Sequence**

INTOXILYZER 8000  
Location:  
Serial Number: 80-002345  
Core Version: 8105.48  
12/11/2015

11:30:42

3 of 8  
JLW  
T84

---

Standard Lot#: 25414100A4  
Last Changed By: A. AUTRET #53546

---

QAS: A. AUTRET #53546  
TUCSON PD

---

Operator: A. AUTRET #53546  
TUCSON PD

---

Subject: SQAP, SQAP  
DOB: 11/11/1987  
Sex: F Weight: 111

---

15 Minute Deprivation Period? Yes

---

Test	g/210L	Time
Air Blank	0.000	11:31:38
Diagnostic Test	Pass	11:32:13
Air Blank	0.000	11:32:40
0.100 Cal Check	RFI*	11:32:54
Air Blank	IPS**	11:33:02

\*RFI Detect  
\*\*Improper Sample

**Not a Successfully Completed Test Sequence**

INTOXILYZER 8000  
Location:  
Serial Number: 80-002345  
Core Version: 8105.48  
12/11/2015

11:33:19

4 of 8  
MA  
Tdy

---

Standard Lot#: 25414100A4  
Last Changed By: A. AUTRET #53546

---

QAS: A. AUTRET #53546  
TUCSON PD

---

Operator: A. AUTRET #53546  
TUCSON PD

---

Subject: SQAP, SQAP  
DOB: 11/11/1987  
Sex: F Weight: 111

---

15 Minute Deprivation Period? Yes

---

Test	g/210L	Time
Air Blank	0.000	11:34:14
Diagnostic Test	RFI*	11:34:37
Air Blank	0.000	11:35:05

\* RFI Detect

Unexpected RFI,  
repeated attempt  
of deficient +  
Invalid sample.

### Not a Successfully Completed Test Sequence

Pursuant to section 28-1327, Arizona Revised Statutes, this document is a certified duplicate of the information contained in computer storage devices of the Tucson Police Department.

INTOXILYZER 8000  
Location:  
Serial Number: 80-002345  
Core Version: 8105.48  
12/11/2015

11:35:09

*5068  
MA  
TSG*

Standard Lot#: 25414100A4  
Last Changed By: A. AUTRET #53546

QAS: A. AUTRET #53546  
TUCSON PD

Operator: A. AUTRET #53546  
TUCSON PD

Subject: SQAP, SQAP  
DOB: 11/11/1987  
Sex: F Weight: 111

15 Minute Deprivation Period? Yes

Test	g/210L	Time
Air Blank	0.000	11:36:02
Diagnostic Test	Pass	11:36:37
Air Blank	0.000	11:37:05
0.100 Cal Check	0.101	11:37:25
Air Blank	0.000	11:37:55
Subject Test	0.262*	11:41:02
Air Blank	0.000	11:41:37
Air Blank	0.000	11:42:04
Subject Test	XXX**	11:42:24
Air Blank	0.000	11:42:59

\*Deficient Sample  
\*\*Invalid Sample  
Begin new deprivation period

**Not a Successfully Completed Test Sequence**

INTOXILYZER 8000

Location:

Serial Number: 80-002345

Core Version: 8105.48

12/11/2015

11:43:54

*6 2/8  
JLH  
TSL*

-----  
Standard Lot#: 25414100A4

Last Changed By: A. AUTRET #53546  
-----

QAS: A. AUTRET #53546

TUCSON PD  
-----

Operator: A. AUTRET #53546

TUCSON PD  
-----

Test	g/210L	Time
Air Blank	0.000	11:44:23
0.100 Cal Check	0.100	11:44:43
Air Blank	0.000	11:45:13

Preventative Maintenance  
Performed -- Timer Reset

EXHIBIT G-2

THIS REPORT PREPARED PURSUANT TO DUTY IMPOSED BY  
A.A.C. R13-10-104(A)

7068  
JW  
TS4  
12-18-2015

ARIZONA DEPARTMENT OF PUBLIC SAFETY

STANDARD QUALITY ASSURANCE PROCEDURES  
INTOXILYZER MODEL 8000

STANDARD CALIBRATION CHECK PROCEDURE

QA Specialist Amy Autret 53546 AGENCY Tucson Police Department  
DATE 12-11-15 TIME 1123  
Intoxilyzer Serial # 80-002345 Location 000

- ( ✓ ) 1. Ensure that gas tank is attached to instrument and contains a standard alcohol concentration solution 0. 100 AC.  
OR  
Pour a standard alcohol concentration solution \_\_\_\_\_ AC, into a clean dry simulator and assemble the simulator. Ensure that a tight seal has been made. Turn on the simulator and allow temperature to reach 34°C + 0.2°C
- ( ✓ ) 2. Intoxilyzer 8000 display reads "PUSH BUTTON TO START"
- ( ✓ ) 3. Go to the "Control Testing Menu". Select "D" for dry control test or "W" for wet control test. After selection is made press ENTER.
- ( ✓ ) 4. Air blank completed.
- ( ✓ ) 5. Calibration check completed. Test results 0. 101 AC.
- ( ✓ ) 6. Air blank completed.
- ( ✓ ) 7. Remove printed record. Attach the record to the completed checklist.

SIGNATURE 

Pursuant to section 28-1327, Arizona Revised Statutes, this document is a certified duplicate of the information contained in computer storage devices of the Tucson Police Department.

8 of 8  
JLD  
BH

INTOXILYZER 8000  
Location:  
Serial Number: 80-002345  
Core Version: 8105.48  
12/11/2015 11:23:51

-----  
Standard Lot#: 25414100A4  
Last Changed By: A. AUTRET #53546  
-----

QAS: A. AUTRET #53546  
TUCSON PD  
-----

Operator: A. AUTRET #53546  
TUCSON PD  
-----

Test	g/210L	Time
Air Blank	0.000	11:24:19
0.100 Cal Check	0.101	11:24:40
Air Blank	0.000	11:25:10

Preventative Maintenance  
Performed -- Timer Reset