



CERTIFICATION by CUSTODIAN of RECORDS  
Tucson Police Department Crime Laboratory

cu  
11-23-07

I hereby certify that these documents are a true and correct copy of the periodic maintenance\* for the Intoxilyzer 8000 Serial Number 80-002759 maintained by the Tucson Police Department Crime Laboratory pursuant to the requirements of the Arizona Department of Public Safety for a quality assurance program.

A quality assurance specialist (QAS) tested the instrument on the following dates. The acceptable accuracy limits, as defined in A.A.C. R13-10-104.A.2, for a 0.100AC solution are 0.090AC to 0.110AC.

Date: 10.23.2007 Cal 1 0.101 AC Cal 2 0.102 AC

The instrument was placed into service on 10.23.2007.

Terry Gallegos

Terry S. Gallegos

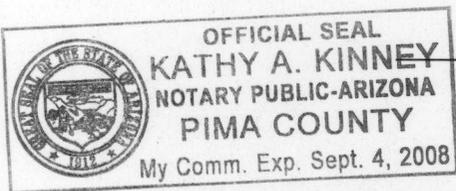
11.21.2007

ADPS QAS Permit # 33169

SUBSCRIBED AND SWORN to before me this 21, day of November, 2007.

Kathy A Kinney

Notary Public



\*Includes documents specified in A.A.C. R13-10-104.A.5

CU  
11-23-07

# CERTIFICATE OF CALIBRATION

## INTOXILYZER® 8000

*This is to certify that the calibration of INTOXILYZER serial number 80-002739, manufactured by CMI, subsidiary of MPD, Inc. of Owensboro, Kentucky, was tested and found to be in compliance with the National Safety Administration Standard for Devices to Measure Breath Alcohol ( F.R., No. 179 48705-48710 Sept. 17, 1993) and with International Recommendation OIML R126 Edition 1998 (E). Calibration solutions are traceable to NIST (NBS) standard material 1828.*

Date 10/5/07

Signed *D. Howard*  
Technician



316 EAST 9TH STREET  
OWENSBORO, KY. 42303

Pursuant to section 28-1327, Arizona Revised Statutes, this document is a certified duplicate of the information contained in computer storage devices of the Tucson Police Department.



TUCSON POLICE DEPARTMENT  
CRIME LABORATORY

CU  
11-23-07

INTOXILYZER SERVICE RECORD

1 of 1  
PL

Intoxilyzer Serial Number: 80-002759

Initial Service Date: 10.23.2007

CMI, Inc. Certificate of Calibration Date: 10.5.2007

EXHIBIT G-4

THIS REPORT PREPARED PURSUANT TO DUTY IMPOSED BY  
A.A.C. R13-10-104(A)

CU  
11-23-07

ARIZONA DEPARTMENT OF PUBLIC SAFETY

STANDARD QUALITY ASSURANCE PROCEDURES  
INTOXILYZER MODEL 8000

1 of 7  
TSh

STANDARD QUALITY ASSURANCE PROCEDURE

QA SPECIALIST Terry Gallegos 28847 AGENCY Tucson Police Department

DATE 10-23-2007 TIME 1715

INTOXILYZER SERIAL # 80-002759 LOCATION Lab

(  ) 1. Display reads "PUSH BUTTON TO START"

DIAGNOSTIC TESTS

- (  ) 1. Clock time check.
- (  ) 2. Date check.

OPERATIONAL TESTS

- (  ) 1. Alcohol-free subject test result 0. 000 AC.
- (  ) 2. Error recognition logic system functioning.  
Not a Successfully Completed Test Sequence printed
- (  ) 3. Proper sample recognition system.  
Not a Successfully Completed Test Sequence printed  
Deficient sample printed.
- (  ) 4. Standard Calibration Check standard 0. 100 AC  
Result: 0. 102 AC

Instrument is operating properly and accurately. YES  NO

COMMENTS

---



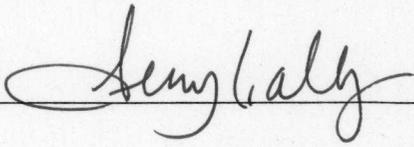
---



---



---

SIGNATURE 

INTOXILYZER 8000  
Location: ARIZONA  
Serial Number : 80-002759  
10/23/2007

17:17:40

cu  
2 of 7  
TS4

---

Standard Lot#: 719802I  
Last Changed By: T. GALLEGOS #28847

---

QAS: T. GALLEGOS #28847  
TUCSON PD CRIME LAB

---

Operator: T. GALLEGOS #28847  
TUCSON PD CRIME LAB

---

Subject: SQAP, SQAP  
DOB: 11/11/1111  
Sex: F Weight: 111

---

15 Minute Deprivation Period? Yes

---

Test	g/210L	Time
Air Blank	0.000	17:18:31
Diagnostic Test	Pass	17:18:59
Air Blank	0.000	17:19:26
0.100 Cal Check	0.103	17:19:45
Air Blank	0.000	17:20:15
Subject Test	0.000	17:22:09
Air Blank	0.000	17:22:36
Five Minute Wait	ABT*	
Air Blank	0.000	17:23:11

\*Sequence Aborted

**Not a Successfully Completed Test Sequence**

Pursuant to section 26-1327, Arizona Revised Statutes, this document is a certified duplicate of the information contained in computer storage devices of the Tucson Police Department.

INTOXILYZER 8000  
Location: ARIZONA  
Serial Number : 80-002759  
10/23/2007

17:25:22

Cu  
3077  
TS4

---

Standard Lot#: 719802I  
Last Changed By: T. GALLEGOS #28847

---

QAS: T. GALLEGOS #28847  
TUCSON PD CRIME LAB

---

Operator: T. GALLEGOS #28847  
TUCSON PD CRIME LAB

---

Subject: SQAP, SQAP  
DOB: 11/11/1111  
Sex: F Weight: 111

---

15 Minute Deprivation Period? Yes

---

Test	g/210L	Time
Air Blank	0.000	17:26:11
Diagnostic Test	Pass	17:26:38
Air Blank	0.000	17:27:05
0.100 Cal Check	0.103	17:27:24
Air Blank	0.000	17:27:54
Subject Test	RFI*	17:28:10
Air Blank	IPS**	17:28:18

\*RFI Detect  
\*\*Improper Sample

**Not a Successfully Completed Test Sequence**

Pursuant to section 28-1527, Arizona Revised Statutes, this document is a certified duplicate of the information contained in computer storage devices of the Tucson Police Department.

INTOXILYZER 8000  
Location: ARIZONA  
Serial Number : 80-002759  
10/23/2007

17:28:22

CU  
4 of 7  
TSh

Standard Lot#: 719802I  
Last Changed By: T. GALLEGOS #28847

QAS: T. GALLEGOS #28847  
TUCSON PD CRIME LAB

Operator: T. GALLEGOS #28847  
TUCSON PD CRIME LAB

Subject: SQAP, SQAP  
DOB: 11/11/1111  
Sex: F Weight: 111

15 Minute Deprivation Period? Yes

Test	g/210L	Time
Air Blank	0.000	17:29:08
Diagnostic Test	Pass	17:29:35
Air Blank	0.000	17:30:02
0.100 Cal Check	0.103	17:30:21
Air Blank	0.000	17:30:51
Subject Test	0.060*	17:33:59
Air Blank	0.000	17:34:31
Air Blank	0.000	17:34:59
Subject Test	XXX**	17:35:16
Air Blank	0.000	17:35:49

\*Deficient Sample

\*\*Invalid Sample

Begin new deprivation period

**Not a Successfully Completed Test Sequence**

Pursuant to section 28-1327, Arizona Revised Statutes, this document is a certified duplicate of the information contained in computer storage devices of the Tucson Police Department.

INTOXILYZER 8000  
Location: ARIZONA  
Serial Number: 80-002759  
10/23/2007 17:36:11

cu  
5077  
T04

-----  
Standard Lot#: 719802I  
Last Changed By: T. GALLEGOS #28847  
-----

QAS: T. GALLEGOS #28847  
TUCSON PD CRIME LAB  
-----

Test	g/210L	Time
Air Blank	0.000	17:36:38
Cal Check	0.102	17:36:57
Air Blank	0.000	17:37:26


  
-----  
Operator's Signature

EXHIBIT G-2

THIS REPORT PREPARED PURSUANT TO DUTY IMPOSED BY  
A.A.C. R13-10-104(A)

CU  
11-23-07  
6077  
TDH

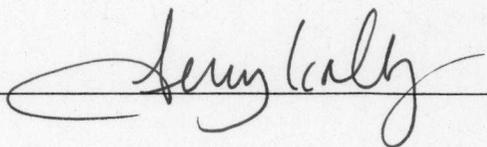
ARIZONA DEPARTMENT OF PUBLIC SAFETY

STANDARD QUALITY ASSURANCE PROCEDURES  
INTOXILYZER MODEL 8000

STANDARD CALIBRATION CHECK PROCEDURE

QA Specialist Terry Gallegos 28847 AGENCY Tucson Police Department  
DATE 10-23-2007 TIME 1715  
Intoxilyzer Serial # 80-002759 Location Lab

- ( ✓ ) 1. Ensure that gas tank is attached to instrument and contains a standard alcohol concentration solution 0. 100 AC.  
OR  
Pour a standard alcohol concentration solution \_\_\_\_\_ AC, into a clean dry simulator and assemble the simulator. Ensure that a tight seal has been made. Turn on the simulator and allow temperature to reach 34°C ± 0.2°C
- ( ✓ ) 2. Intoxilyzer 8000 display reads "PUSH BUTTON TO START"
- ( ✓ ) 3. Go to the "Control Testing Menu". Select "D" for dry control test or "W" for wet control test. After selection is made press ENTER.
- ( ✓ ) 4. Air blank completed.
- ( ✓ ) 5. Calibration check completed. Test results 0. 101 AC.
- ( ✓ ) 6. Air blank completed.
- ( ✓ ) 7. Remove printed record. Attach the record to the completed checklist.

SIGNATURE 

DPS Form Exh G-2 (Rev. 05-01)

INTOXILYZER 8000  
Location: ARIZONA  
Serial Number: 80-002759  
10/23/2007 17:15:41

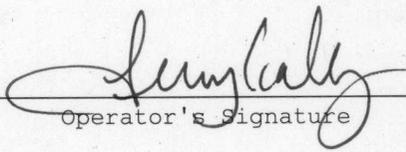
*cl*

*7057  
TS4*

-----  
Standard Lot#: 719802I  
Last Changed By: T. GALLEGOS #28847  
-----

QAS: T. GALLEGOS #28847  
TUCSON PD CRIME LAB  
-----

Test	g/210L	Time
Air Blank	0.000	17:16:08
Cal Check	0.101	17:16:27
Air Blank	0.000	17:16:57

  
-----  
Operator's Signature