



CERTIFICATION by CUSTODIAN of RECORDS

Tucson Police Department Crime Laboratory
270 S. Stone Avenue Tucson, AZ 85701-1917

I hereby certify that these documents are a true and correct copy of the periodic maintenance* for the Intoxilyzer 8000 Serial Number 80-002759 maintained by the Tucson Police Department Crime Laboratory pursuant to the requirements of the Arizona Department of Public Safety for a quality assurance program.

TS4
12-24-08

A quality assurance specialist (QAS) tested the instrument on the following dates. The acceptable accuracy limits, as defined in A.A.C. R13-10-104.A.2, for a 0.100AC solution are 0.090AC to 0.110AC.

Date: 12-18-08 Cal 1 0.096 AC Cal 2 0.097 AC

Between the dates of 12-2-08 and 12-18-08 the instrument was operating properly and accurately.

The instrument was taken out of service for repair on N/A.
The instrument was returned to service on N/A.

Clare Conley

Clare L. Conley


12-23-08

ADPS QAS Permit # 33314

SUBSCRIBED AND SWORN to before me this 23, day of December, 2008.

A.M. Hernández

Notary Public

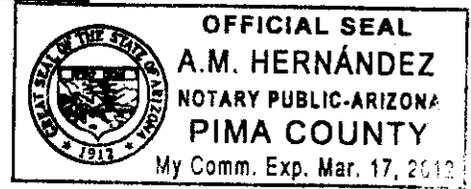

*Includes documents specified in A.A.C. R13-10-104.A.5

EXHIBIT G-4

THIS REPORT PREPARED PURSUANT TO DUTY IMPOSED BY
A.A.C. R13-10-104(A)

ARIZONA DEPARTMENT OF PUBLIC SAFETY
STANDARD QUALITY ASSURANCE PROCEDURES
INTOXILYZER MODEL 8000
STANDARD QUALITY ASSURANCE PROCEDURE

107
On
TS4
12-24-08

QA SPECIALIST Clare Conley AGENCY Tucson Police Department

DATE 12-18-08 TIME 0936

INTOXILYZER SERIAL # 80-002759 LOCATION DUI HQ ODW

(✓) 1. Display reads "PUSH BUTTON TO START"

DIAGNOSTIC TESTS

(✓) 1. Clock time check.

(✓) 2. Date check.

OPERATIONAL TESTS

(✓) 1. Alcohol-free subject test result 0. 000 AC.

(✓) 2. Error recognition logic system functioning.
Not a Successfully Completed Test Sequence printed

(✓) 3. Proper sample recognition system.
Not a Successfully Completed Test Sequence printed
Deficient sample printed.

(✓) 4. Standard Calibration Check standard 0. 100 AC
Result: 0. 097 AC

Instrument is operating properly and accurately. YES NO

COMMENTS None.

SIGNATURE Clare Conley

INTOXILYZER 8000
Location: TUCSON PD
Serial Number : 80-002759
12/18/2008

09:38:04

207
C
154

Standard Lot#: 725401I
Last Changed By: S. CIONE - #50616

QAS: C. CONLEY #34517
TUCSON PD

Operator: C. CONLEY #34517
TUCSON PD

Subject: TEST, SQAP
DOB: 11/11/1111
Sex: M Weight: 111

15 Minute Deprivation Period? Yes

Test	g/210L	Time
Air Blank	0.000	09:38:49
Diagnostic Test	Pass	09:39:16
Air Blank	0.000	09:39:43
0.100 Cal Check	0.097	09:40:02
Air Blank	0.000	09:40:32
Subject Test	0.000	09:40:50
Air Blank	ABT*	09:40:56
Air Blank	0.000	09:41:24

*Sequence Aborted

Not a Successfully Completed Test Sequence

Pursuant to section 28-1327, Arizona Revised Statutes, this document is a certified duplicate of the information contained in computer storage devices of the Tucson Police Department.

INTOXILYZER 8000
Location: TUCSON PD
Serial Number : 80-002759
12/18/2008

09:48:33

3067
Cu
AH

Standard Lot#: 725401I
Last Changed By: S. CIONE - #50616

QAS: C. CONLEY #34517
TUCSON PD

Operator: C. CONLEY #34517
TUCSON PD

Subject: TEST, SQAP
DOB: 11/11/1111
Sex: M Weight: 111

15 Minute Deprivation Period? Yes

Test	g/210L	Time
Air Blank	RFI*	09:49:09
Air Blank	IPS**	09:49:18

*RFI Detect
**Improper Sample

Not a Successfully Completed Test Sequence

Pursuant to section 28-1327, Arizona Revised Statutes, this document is a certified duplicate of the information contained in computer storage devices of the Tucson Police Department.

INTOXILYZER 8000
Location: TUCSON PD
Serial Number : 80-002759
12/18/2008

09:49:53

487
cu
154

Standard Lot#: 725401I
Last Changed By: S. CIONE - #50616

QAS: C. CONLEY #34517
TUCSON PD

Operator: C. CONLEY #34517
TUCSON PD

Subject: TEST, SQAP
DOB: 11/11/1111
Sex: M Weight: 111

15 Minute Deprivation Period? Yes

Test	g/210L	Time
Air Blank	0.000	09:50:42
Diagnostic Test	Pass	09:51:09
Air Blank	0.000	09:51:37
0.100 Cal Check	0.097	09:51:55
Air Blank	0.000	09:52:25
Subject Test	0.179*	09:55:33
Air Blank	0.000	09:56:05
Air Blank	0.000	09:56:33
Subject Test	XXX**	09:57:16
Air Blank	0.000	09:57:50

*Deficient Sample

**Invalid Sample

Begin new deprivation period

Not a Successfully Completed Test Sequence

INTOXILYZER 8000
Location: TUCSON PD
Serial Number: 80-002759
12/18/2008

09:58:05

Standard Lot#: 725401I
Last Changed By: S. CIONE #50616

QAS: C. CONLEY #34517
TUCSON PD

Test	g/210L	Time
Air Blank	0.000	09:58:32
Cal Check	0.097	09:58:51
Air Blank	0.000	09:59:21

Clare Conley

Operator's Signature

5 of 7
cu
TS4

EXHIBIT G-2

THIS REPORT PREPARED PURSUANT TO DUTY IMPOSED BY
A.A.C. R13-10-104(A)

ARIZONA DEPARTMENT OF PUBLIC SAFETY

STANDARD QUALITY ASSURANCE PROCEDURES
INTOXILYZER MODEL 8000

STANDARD CALIBRATION CHECK PROCEDURE

b587
Cu
12-24-08

QA Specialist Clare Conley AGENCY Tucson Police Department
DATE 12-18-08 TIME 0936
Intoxilyzer Serial # 80-002759 Location ODW DM HQ

- (/) 1. Ensure that gas tank is attached to instrument and contains a standard alcohol concentration solution 0. 100 AC.
OR
Pour a standard alcohol concentration solution _____ AC, into a clean dry simulator and assemble the simulator. Ensure that a tight seal has been made. Turn on the simulator and allow temperature to reach $34^{\circ}\text{C} \pm 0.2^{\circ}\text{C}$
- (/) 2. Intoxilyzer 8000 display reads "PUSH BUTTON TO START"
- (/) 3. Go to the "Control Testing Menu". Select "D" for dry control test or "W" for wet control test. After selection is made press ENTER.
- (/) 4. Air blank completed.
- (/) 5. Calibration check completed. Test results 0. 096 AC.
- (/) 6. Air blank completed.
- (/) 7. Remove printed record. Attach the record to the completed checklist.

SIGNATURE Clare Conley

DPS Form Exh G-2 (Rev. 05-01)

Pursuant to section 28-1327, Arizona Revised Statutes, this document is a certified duplicate of the information contained in computer storage devices of the Tucson Police Department.

INTOXILYZER 8000
Location: TUCSON PD
Serial Number: 80-002759
12/18/2008 09:36:42

7567
Cu
154

Standard Lot#: 725401I
Last Changed By: S. CIONE #50616

QAS: C. CONLEY #34517
TUCSON PD

Test	g/210L	Time
Air Blank	0.000	09:37:09
Cal Check	0.096	09:37:28
Air Blank	0.000	09:37:58

Clare Conley
Operator's Signature