



CERTIFICATION by CUSTODIAN of RECORDS

Tucson Police Department Crime Laboratory
270 S. Stone Avenue Tucson, AZ 85701-1917

TS4
7-28-09

I hereby certify that these documents are a true and correct copy of the periodic maintenance* for the Intoxilyzer 8000 Serial Number 80-002759 maintained by the Tucson Police Department Crime Laboratory pursuant to the requirements of the Arizona Department of Public Safety for a quality assurance program.

A quality assurance specialist (QAS) tested the instrument on the following dates. The acceptable accuracy limits, as defined in A.A.C. R13-10-104.A.2, for a 0.100AC solution are 0.090AC to 0.110AC.

Date: 07/27/09 Cal 1 0.096 AC Cal 2 0.097 AC

Between the dates of 06/26/09 and 07/27/09 the instrument was operating properly and accurately.

The instrument was taken out of service for repair on .
The instrument was returned to service on .

Cheryl K. Straub

Cheryl K. Straub


07/28/09

ADPS QAS Permit # 33408

SUBSCRIBED AND SWORN to before me this 28, day of July, 20 09.

A.M. Hernandez

Notary Public

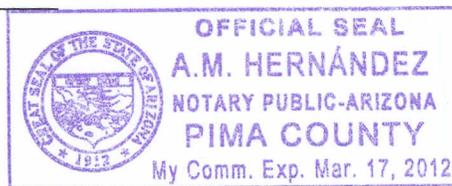

*Includes documents specified in A.A.C. R13-10-104.A.5

1 of 7
CS

THIS REPORT PREPARED PURSUANT TO DUTY IMPOSED BY
A.A.C. R13-10-104(A)

ARIZONA DEPARTMENT OF PUBLIC SAFETY

STANDARD QUALITY ASSURANCE PROCEDURES
INTOXILYZER MODEL 8000

TSB
7-28-09

STANDARD QUALITY ASSURANCE PROCEDURE

QA SPECIALIST Cheryl Straub AGENCY Tucson Police Department

DATE 07/27/09 TIME 16:52

INTOXILYZER SERIAL # 80-002759 LOCATION TEAM 4

() 1. Display reads "PUSH BUTTON TO START"

DIAGNOSTIC TESTS

- () 1. Clock time check.
- () 2. Date check.

OPERATIONAL TESTS

- () 1. Alcohol-free subject test result 0. 000 AC.
- () 2. Error recognition logic system functioning.
Not a Successfully Completed Test Sequence printed
- () 3. Proper sample recognition system.
Not a Successfully Completed Test Sequence printed
Deficient sample printed.
- () 4. Standard Calibration Check standard 0. 100 AC
Result: 0. 097 AC

Instrument is operating properly and accurately. YES NO

COMMENTS

SIGNATURE

Cheryl Straub

277
CS

INTOXILYZER 8000
Location: TUCSON PD
Serial Number : 80-002759
07/27/2009

16:55:38

SM

Standard Lot#: 808101G
Last Changed By: S. CIONE #50616

QAS: C. STRAUB #50772
TUCSON PD

Operator: C. STRAUB #50772
TUCSON PD

Subject: SQAP, SQAP
DOB: 11/11/1111
Sex: F Weight: 111

15 Minute Deprivation Period? Yes

Test	g/210L	Time
Air Blank	0.000	16:56:31
Diagnostic Test	Pass	16:56:59
Air Blank	0.000	16:57:26
0.100 Cal Check	0.096	16:57:45
Air Blank	0.000	16:58:14
Subject Test	0.000	16:58:33
Air Blank	ABT*	16:58:40
Air Blank	0.000	16:59:08

*Sequence Aborted

Not a Successfully Completed Test Sequence

377
CS

INTOXILYZER 8000
Location: TUCSON PD
Serial Number : 80-002759
07/27/2009

16:59:16

SM

Standard Lot#: 808101G
Last Changed By: S. CIONE #50616

QAS: C. STRAUB #50772
TUCSON PD

Operator: C. STRAUB #50772
TUCSON PD

Subject: SQAP, SQAP
DOB: 11/11/1111
Sex: F Weight: 111

15 Minute Deprivation Period? Yes

Test	g/210L	Time
Air Blank	RFI*	16:59:51
Air Blank	IPS**	16:59:59

*RFI Detect
**Improper Sample

Not a Successfully Completed Test Sequence

487
CS

INTOXILYZER 8000
Location: TUCSON PD
Serial Number : 80-002759
07/27/2009

17:00:19

154

Standard Lot#: 808101G
Last Changed By: S. CIONE #50616

QAS: C. STRAUB #50772
TUCSON PD

Operator: C. STRAUB #50772
TUCSON PD

Subject: SQAP, SQAP
DOB: 11/11/1111
Sex: F Weight: 111

15 Minute Deprivation Period? Yes

Test	g/210L	Time
Air Blank	0.000	17:01:11
Diagnostic Test	Pass	17:01:38
Air Blank	0.000	17:02:06
0.100 Cal Check	0.097	17:02:25
Air Blank	0.000	17:02:54
Subject Test	0.189*	17:06:03
Air Blank	0.000	17:06:35
Air Blank	0.000	17:07:02
Subject Test	XXX**	17:07:25
Air Blank	0.000	17:07:59

*Deficient Sample

**Invalid Sample

Begin new deprivation period

Not a Successfully Completed Test Sequence

587
CS

INTOXILYZER 8000
Location: TUCSON PD
Serial Number: 80-002759
07/27/2009 17:09:13

PS

Standard Lot#: 808101G
Last Changed By: S. CIONE #50616

QAS: C. STRAUB #50772
TUCSON PD

Test	g/210L	Time
Air Blank	0.000	17:09:40
Cal Check	0.097	17:09:59
Air Blank	0.000	17:10:29



Operator's Signature

697
CS

THIS REPORT PREPARED PURSUANT TO DUTY IMPOSED BY
A.A.C. R13-10-104(A)

ARIZONA DEPARTMENT OF PUBLIC SAFETY
STANDARD QUALITY ASSURANCE PROCEDURES
INTOXILYZER MODEL 8000
STANDARD CALIBRATION CHECK PROCEDURE

154
7-28-09

QA Specialist Cheryl STRAUB AGENCY Tucson Police Department
DATE 07/27/09 TIME 16:52
Intoxilyzer Serial # 80-002759 Location TEAM 4

- (✓) 1. Ensure that gas tank is attached to instrument and contains a standard alcohol concentration solution 0. 100 AC.
OR
Pour a standard alcohol concentration solution _____ AC, into a clean dry simulator and assemble the simulator. Ensure that a tight seal has been made. Turn on the simulator and allow temperature to reach 34°C ± 0.2°C
- (✓) 2. Intoxilyzer 8000 display reads "PUSH BUTTON TO START"
- (✓) 3. Go to the "Control Testing Menu". Select "D" for dry control test or "W" for wet control test. After selection is made press ENTER.
- (✓) 4. Air blank completed.
- (✓) 5. Calibration check completed. Test results 0. 094 AC.
- (✓) 6. Air blank completed.
- (✓) 7. Remove printed record. Attach the record to the completed checklist.

SIGNATURE Cheryl Straub

Pursuant to section 28-1327, Arizona Revised Statutes, this document is a certified duplicate of the information contained in computer storage devices of the Tucson Police Department.

7 of 7
CS

INTOXILYZER 8000
Location: TUCSON PD
Serial Number: 80-002759
07/27/2009 16:52:51

AM

Standard Lot#: 808101G
Last Changed By: S. CIONE #50616

QAS: C. STRAUB #50772
TUCSON PD

Test	g/210L	Time
Air Blank	0.000	16:53:19
Cal Check	0.096	16:53:38
Air Blank	0.000	16:54:07

Cheryl Straub

Operator's Signature