



CERTIFICATION by CUSTODIAN of RECORDS

Tucson Police Department Crime Laboratory  
270 S. Stone Avenue Tucson, AZ 85701-1917

TSY  
7-6-2010

I hereby certify that these documents are a true and correct copy of the periodic maintenance\* for the Intoxilyzer 8000 Serial Number 80-002759 maintained by the Tucson Police Department Crime Laboratory pursuant to the requirements of the Arizona Department of Public Safety for a quality assurance program.

A quality assurance specialist (QAS) tested the instrument on the following dates. The acceptable accuracy limits, as defined in A.A.C. R13-10-104.A.2, for a 0.100AC solution are 0.090AC to 0.110AC.

Date: 07/01/10 Cal 1 0.099 AC Cal 2 0.099 AC

Between the dates of 06/03/10 and 07/01/10 the instrument was operating properly and accurately.

The instrument was taken out of service for repair on N/A.  
The instrument was returned to service on N/A.

Cheryl K. Straub

Cheryl K. Straub


07/01/10

ADPS QAS Permit # 33408

SUBSCRIBED AND SWORN to before me this 1, day of July, 2010.

A.M. Hernandez

Notary Public

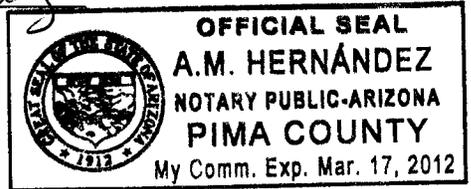

\*Includes documents specified in A.A.C. R13-10-104.A.5

197  
CS

EXHIBIT G-4

THIS REPORT PREPARED PURSUANT TO DUTY IMPOSED BY  
A.A.C. R13-10-104(A)

ARIZONA DEPARTMENT OF PUBLIC SAFETY

STANDARD QUALITY ASSURANCE PROCEDURES  
INTOXILYZER MODEL 8000

STANDARD QUALITY ASSURANCE PROCEDURE

TSY  
7-6-2010

QA SPECIALIST Cheryl STRAUB AGENCY Tucson Police Department

DATE 07/01/10 TIME 07:05

INTOXILYZER SERIAL # 80-002759 LOCATION TEAM 4

(  ) 1. Display reads "PUSH BUTTON TO START"

DIAGNOSTIC TESTS

- (  ) 1. Clock time check.
- (  ) 2. Date check.

OPERATIONAL TESTS

- (  ) 1. Alcohol-free subject test result 0. 060 AC.
- ( ) 2. Error recognition logic system functioning.  
Not a Successfully Completed Test Sequence printed
- (  ) 3. Proper sample recognition system.  
Not a Successfully Completed Test Sequence printed  
Deficient sample printed.
- (  ) 4. Standard Calibration Check standard 0. 100 AC  
Result: 0. 099 AC

Instrument is operating properly and accurately. YES  NO

COMMENTS

---



---



---



---

SIGNATURE

Cheryl Straub

Pursuant to section 28-1327, Arizona Revised Statutes, this document is a certified duplicate of the information contained in computer storage devices of the Tucson Police Department.

277  
CS

TS4

INTOXILYZER 8000

Location:

Serial Number : 80-002759

07/01/2010

07:09:17

Standard Lot#: 719919

Last Changed By: C. CONLEY

#34517

QAS: C. STRAUB

#50772

TUCSON PD

Operator: C. STRAUB

#50772

TUCSON PD

Subject: SQAP, SQAP

DOB: 11/11/1111

Sex: F

Weight: 111

15 Minute Deprivation Period? Yes

Test	g/210L	Time
Air Blank	0.000	07:10:15
Diagnostic Test	Pass	07:10:43
Air Blank	0.000	07:11:10
0.100 Cal Check	0.099	07:11:29
Air Blank	0.000	07:11:58
Subject Test	0.000	07:12:17
Air Blank	ABT*	07:12:25
Air Blank	0.000	07:12:53

\*Sequence Aborted

**Not a Successfully Completed Test Sequence**

377  
CS

TS4

INTOXILYZER 8000  
Location:  
Serial Number : 80-002759  
07/01/2010 07:12:58

---

Standard Lot#: 719919  
Last Changed By: C. CONLEY #34517

---

QAS: C. STRAUB #50772  
TUCSON PD

---

Operator: C. STRAUB #50772  
TUCSON PD

---

Subject: SQAP, SQAP  
DOB: 11/11/1111  
Sex: F Weight: 111

---

15 Minute Deprivation Period? Yes

---

Test	g/210L	Time
Air Blank	RFI*	07:13:40
Air Blank	IPS**	07:13:49

\*RFI Detect  
\*\*Improper Sample

**Not a Successfully Completed Test Sequence**

Pursuant to section 28-1327, Arizona Revised Statutes, this document is a certified duplicate of the information contained in computer storage devices of the Tucson Police Department.

477  
CS

784

INTOXILYZER 8000

Location:

Serial Number : 80-002759

07/01/2010

07:13:57

Standard Lot#: 719919

Last Changed By: C. CONLEY

#34517

QAS: C. STRAUB

#50772

TUCSON PD

Operator: C. STRAUB

#50772

TUCSON PD

Subject: SQAP, SQAP

DOB: 11/11/1111

Sex: F

Weight: 111

15 Minute Deprivation Period? Yes

Test	g/210L	Time
Air Blank	0.000	07:14:55
Diagnostic Test	Pass	07:15:23
Air Blank	0.000	07:15:50
0.100 Cal Check	0.098	07:16:09
Air Blank	0.000	07:16:38
Subject Test	0.102*	07:19:47
Air Blank	0.000	07:20:19
Air Blank	0.000	07:20:46
Subject Test	XXX**	07:21:17
Air Blank	0.000	07:21:51

\*Deficient Sample

\*\*Invalid Sample

Begin new deprivation period

**Not a Successfully Completed Test Sequence**

577  
CS


TS4

INTOXILYZER 8000  
Location:  
Serial Number: 80-002759  
07/01/2010 07:22:24

-----  
Standard Lot#: 719919  
Last Changed By: C. CONLEY #34517  
-----

QAS: C. STRAUB #50772  
TUCSON PD  
-----

Test	g/210L	Time
Air Blank	0.000	07:22:51
Cal Check	0.099	07:23:10
Air Blank	0.000	07:23:40



\_\_\_\_\_  
Operator's Signature

EXHIBIT G-2

THIS REPORT PREPARED PURSUANT TO DUTY IMPOSED BY  
A.A.C. R13-10-104(A)

787 CS  
CS  
687 CS

ARIZONA DEPARTMENT OF PUBLIC SAFETY  
STANDARD QUALITY ASSURANCE PROCEDURES  
INTOXILYZER MODEL 8000  
STANDARD CALIBRATION CHECK PROCEDURE

TSY  
7-6-2010

QA Specialist Cheryl Straub AGENCY Tucson Police Department  
DATE 07/01/10 TIME 07:05  
Intoxilyzer Serial # 80-002759 Location TEAM 4

- ( ✓ ) 1. Ensure that gas tank is attached to instrument and contains a standard alcohol concentration solution 0. 100 AC.  
OR  
Pour a standard alcohol concentration solution N/A AC, into a clean dry simulator and assemble the simulator. Ensure that a tight seal has been made. Turn on the simulator and allow temperature to reach 34°C ± 0.2°C
- ( ✓ ) 2. Intoxilyzer 8000 display reads "PUSH BUTTON TO START"
- ( ✓ ) 3. Go to the "Control Testing Menu". Select "D" for dry control test or "W" for wet control test. After selection is made press ENTER.
- ( ✓ ) 4. Air blank completed.
- ( ✓ ) 5. Calibration check completed. Test results 0. 099 AC.
- ( ✓ ) 6. Air blank completed.
- ( ✓ ) 7. Remove printed record. Attach the record to the completed checklist.

SIGNATURE Cheryl Straub

DPS Form Exh G-2 (Rev. 05-01)

~~677~~ CS  
CS  
777 CS

INTOXILYZER 8000  
Location:  
Serial Number: 80-002759  
07/01/2010


07:05:05

104

-----  
Standard Lot#: 719919  
Last Changed By: C. CONLEY #34517  
-----

QAS: C. STRAUB #50772  
TUCSON PD  
-----

Test	g/210L	Time
Air Blank	0.000	07:05:32
Cal Check	0.099	07:05:51
Air Blank	0.000	07:06:20



Operator's Signature