



CERTIFICATION by CUSTODIAN of RECORDS

Tucson Police Department Crime Laboratory  
270 S. Stone Avenue Tucson, AZ 85701-1917

BSy  
9.2.2010

I hereby certify that these documents are a true and correct copy of the periodic maintenance\* for the Intoxilyzer 8000 Serial Number 80-002759 maintained by the Tucson Police Department Crime Laboratory pursuant to the requirements of the Arizona Department of Public Safety for a quality assurance program.

A quality assurance specialist (QAS) tested the instrument on the following dates. The acceptable accuracy limits, as defined in A.A.C. R13-10-104.A.2, for a 0.100AC solution are 0.090AC to 0.110AC.

Date: 08/26/10 Cal 1 0.098 AC Cal 2 0.099 AC

Between the dates of 07/29/10 and 08/26/10 the instrument was operating properly and accurately.

The instrument was taken out of service for repair on N/A.  
The instrument was returned to service on N/A.

Cheryl K. Straub

Cheryl K. Straub


08/31/10

ADPS QAS Permit # 33408

SUBSCRIBED AND SWORN to before me this 31, day of August, 2010.

A.M. Hernandez

Notary Public

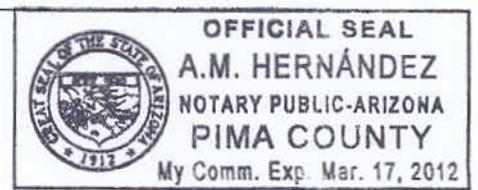

\*Includes documents specified in A.A.C. R13-10-104.A.5

187  
CS

THIS REPORT PREPARED PURSUANT TO DUTY IMPOSED BY  
A.A.C. R13-10-104(A)

ARIZONA DEPARTMENT OF PUBLIC SAFETY  
STANDARD QUALITY ASSURANCE PROCEDURES  
INTOXILYZER MODEL 8000  
STANDARD QUALITY ASSURANCE PROCEDURE

TS4  
9-2-2010

QA SPECIALIST Cheryl STRAUB AGENCY Tucson Police Department  
DATE 08/26/10 TIME 06:09  
INTOXILYZER SERIAL # 80-002759 LOCATION TEAM 4

( ✓ ) 1. Display reads "PUSH BUTTON TO START"

DIAGNOSTIC TESTS

- ( ✓ ) 1. Clock time check.
- ( ✓ ) 2. Date check.

OPERATIONAL TESTS

- ( ✓ ) 1. Alcohol-free subject test result 0. 000 AC.
- ( ✓ ) 2. Error recognition logic system functioning.  
Not a Successfully Completed Test Sequence printed
- ( ✓ ) 3. Proper sample recognition system.  
Not a Successfully Completed Test Sequence printed  
Deficient sample printed.
- ( ✓ ) 4. Standard Calibration Check standard 0. 100 AC.  
Result: 0. 099 AC

Instrument is operating properly and accurately. YES  NO

COMMENTS  
\_\_\_\_\_  
\_\_\_\_\_  
\_\_\_\_\_

SIGNATURE Cheryl Straub

Pursuant to section 28-1327, Arizona Revised Statutes, this document is a certified duplicate of the information contained in computer storage devices of the Tucson Police Department.

277  
CS

TS4

INTOXILYZER 8000  
Location:  
Serial Number : 80-002759  
08/26/2010 06:11:52

Standard Lot#: 719919  
Last Changed By: C. CONLEY #34517

QAS: C. STRAUB #50772  
TUCSON PD

Operator: C. STRAUB #50772  
TUCSON PD

Subject: SQAP, SQAP  
DOB: 11/11/1111  
Sex: F Weight: 111

15 Minute Deprivation Period? Yes

| Test            | g/210L | Time     |
|-----------------|--------|----------|
| Air Blank       | 0.000  | 06:12:47 |
| Diagnostic Test | Pass   | 06:13:14 |
| Air Blank       | 0.000  | 06:13:41 |
| 0.100 Cal Check | 0.098  | 06:14:00 |
| Air Blank       | 0.000  | 06:14:30 |
| Subject Test    | 0.000  | 06:14:50 |
| Air Blank       | ABT*   | 06:14:57 |
| Air Blank       | 0.000  | 06:15:26 |

\*Sequence Aborted

**Not a Successfully Completed Test Sequence**

Pursuant to section 28-1327, Arizona Revised Statutes, this document is a certified duplicate of the information contained in computer storage devices of the Tucson Police Department.

337  
CS

INTOXILYZER 8000

Location:

Serial Number : 80-002759

08/26/2010

06:15:31

TS4

Standard Lot#: 719919

Last Changed By: C. CONLEY.

#34517

OAS: C. STRAUB

#50772

TUCSON PD

Operator: C. STRAUB

#50772

TUCSON PD

Subject: SOAP, SOAP

DOB: 11/11/1111

Sex: F

Weight: 111

15 Minute Deprivation Period? Yes

| Test      | g/210L | Time     |
|-----------|--------|----------|
| Air Blank | RFI*   | 06:16:09 |
| Air Blank | IPS**  | 06:16:18 |

\*RFI Detect

\*\*Improper Sample

**Not a Successfully Completed Test Sequence**

Pursuant to section 28-1327, Arizona Revised Statutes, this document is a certified duplicate of the information contained in computer storage devices of the Tucson Police Department.

477  
CS

TJ4

INTOXILYZER 8000

Location:

Serial Number : 80-002759

08/26/2010

06:16:31

Standard Lot#: 719919

Last Changed By: C. CONLEY.

#34517

QAS: C. STRAUB

#50772

TUCSON PD

Operator: C. STRAUB

#50772

TUCSON PD

Subject: SQAP, SQAP

DOB: 11/11/1111

Sex: F

Weight: 111

15 Minute Deprivation Period? Yes

| Test            | g/210L | Time     |
|-----------------|--------|----------|
| Air Blank       | 0.000  | 06:17:23 |
| Diagnostic Test | Pass   | 06:17:51 |
| Air Blank       | 0.000  | 06:18:18 |
| 0.100 Cal Check | 0.098  | 06:18:37 |
| Air Blank       | 0.000  | 06:19:07 |
| Subject Test    | 0.461* | 06:22:15 |
| Air Blank       | 0.000  | 06:22:51 |
| Air Blank       | 0.000  | 06:23:18 |
| Subject Test    | XXX**  | 06:23:55 |
| Air Blank       | 0.000  | 06:24:28 |

\*Deficient Sample

\*\*Invalid Sample

Begin new deprivation period

### Not a Successfully Completed Test Sequence

577  
CS

INTOXILYZER 8000

Location:

Serial Number: 80-002759

08/26/2010

06:25:05

TS4


-----  
Standard Lot#: 719919

Last Changed By: C. CONLEY #34517

-----  
QAS: C. STRAUB #50772

TUCSON PD  
-----

| Test      | g/210L | Time     |
|-----------|--------|----------|
| Air Blank | 0.000  | 06:25:33 |
| Cal Check | 0.099  | 06:25:51 |
| Air Blank | 0.000  | 06:26:21 |



\_\_\_\_\_  
Operator's Signature

THIS REPORT PREPARED PURSUANT TO DUTY IMPOSED BY  
A.A.C. R13-10-104(A)

ARIZONA DEPARTMENT OF PUBLIC SAFETY

STANDARD QUALITY ASSURANCE PROCEDURES  
INTOXILYZER MODEL 8000

STANDARD CALIBRATION CHECK PROCEDURE

TSY  
9.2.2010

QA Specialist Cheryl STRAUB AGENCY Tucson Police Department  
DATE 08/26/10 TIME 06:09  
Intoxilyzer Serial # 80-002759 Location TEAM 4

- ( ✓ ) 1. Ensure that gas tank is attached to instrument and contains a standard alcohol concentration solution 0. 100 AC.  
OR  
Pour a standard alcohol concentration solution N/A AC, into a clean dry simulator and assemble the simulator. Ensure that a tight seal has been made. Turn on the simulator and allow temperature to reach  $34^{\circ}\text{C} \pm 0.2^{\circ}\text{C}$
- ( ✓ ) 2. Intoxilyzer 8000 display reads "PUSH BUTTON TO START"
- ( ✓ ) 3. Go to the "Control Testing Menu". Select "D" for dry control test or "W" for wet control test. After selection is made press ENTER.
- ( ✓ ) 4. Air blank completed.
- ( ✓ ) 5. Calibration check completed. Test results 0. 098 AC.
- ( ✓ ) 6. Air blank completed.
- ( ✓ ) 7. Remove printed record. Attach the record to the completed checklist.

SIGNATURE

Cheryl Straub

DPS Form Exh G-2 (Rev. 05-01)

787  
CS


TS4

INTOXILYZER 8000  
Location:  
Serial Number: 80-002759  
08/26/2010 06:09:34

-----  
Standard Lot#: 719919  
Last Changed By: C. CONLEY #34517  
-----

QAS: C. STRAUB #50772  
TUCSON PD  
-----

| Test      | g/210L | Time     |
|-----------|--------|----------|
| Air Blank | 0.000  | 06:10:01 |
| Cal Check | 0.098  | 06:10:20 |
| Air Blank | 0.000  | 06:10:49 |



Operator's Signature