



CERTIFICATION by CUSTODIAN of RECORDS
 Tucson Police Department Crime Laboratory
 270 S. Stone Avenue Tucson, AZ 85701-1917

TS4
 9.27-2010

I hereby certify that these documents are a true and correct copy of the periodic maintenance* for the Intoxilyzer 8000 Serial Number 80-002759 maintained by the Tucson Police Department Crime Laboratory pursuant to the requirements of the Arizona Department of Public Safety for a quality assurance program.

A quality assurance specialist (QAS) tested the instrument on the following dates. The acceptable accuracy limits, as defined in A.A.C. R13-10-104.A.2, for a 0.100AC solution are 0.090AC to 0.110AC.

Date: 09/23/10 Cal 1 0.098 AC Cal 2 0.097 AC

Between the dates of 08/26/10 and 09/23/10 the instrument was operating properly and accurately.

The instrument was taken out of service for repair on N/A.
 The instrument was returned to service on N/A.

Cheryl K. Straub

Cheryl K. Straub


09/27/10

ADPS QAS Permit # 33408

SUBSCRIBED AND SWORN to before me this 27, day of September, 2010.

A.M. Hernandez

Notary Public

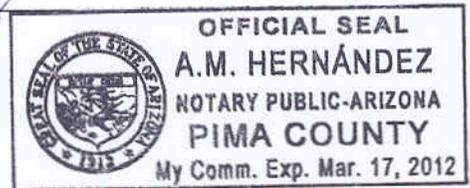

*Includes documents specified in A.A.C. R13-10-104.A.5

177
CS

THIS REPORT PREPARED PURSUANT TO DUTY IMPOSED BY
A.A.C. R13-10-104(A)

ARIZONA DEPARTMENT OF PUBLIC SAFETY

STANDARD QUALITY ASSURANCE PROCEDURES
INTOXILYZER MODEL 8000

STANDARD QUALITY ASSURANCE PROCEDURE

BH
9-27-2010

QA SPECIALIST Cheryl STRAUB AGENCY Tucson Police Department

DATE 09/23/10 TIME 05:46

INTOXILYZER SERIAL # 80-002759 LOCATION TEAM 4

(✓) 1. Display reads "PUSH BUTTON TO START"

DIAGNOSTIC TESTS

- (✓) 1. Clock time check.
- (✓) 2. Date check.

OPERATIONAL TESTS

- (✓) 1. Alcohol-free subject test result 0. 000 AC.
- (✓) 2. Error recognition logic system functioning.
Not a Successfully Completed Test Sequence printed
- (✓) 3. Proper sample recognition system.
Not a Successfully Completed Test Sequence printed
Deficient sample printed.
- (✓) 4. Standard Calibration Check standard 0. 100 AC
Result: 0. 097 AC

Instrument is operating properly and accurately. YES NO

COMMENTS

SIGNATURE Cheryl Straub

277
CS

INTOXILYZER 8000

Location:

Serial Number : 80-002759

09/23/2010

05:49:39

B4

Standard Lot#: 719919

Last Changed By: C. CONLEY-

#34517

QAS: C. STRAUB

#50772

TUCSON PD

Operator: C. STRAUB

#50772

TUCSON PD

Subject: SQAP, SQAP

DOB: 11/11/1111

Sex: F

Weight: 111

15 Minute Deprivation Period? Yes

Test	g/210L	Time
Air Blank	0.000	05:50:33
Diagnostic Test	Pass	05:51:01
Air Blank	0.000	05:51:28
0.100 Cal Check	0.099	05:51:47
Air Blank	0.000	05:52:16
Subject Test	0.000	05:52:40
Air Blank	ABT*	05:52:48
Air Blank	0.000	05:53:16

*Sequence Aborted

Not a Successfully Completed Test Sequence

Pursuant to section 28-1327, Arizona Revised Statutes, this document is a certified duplicate of the information contained in computer storage devices of the Tucson Police Department.

377
CS

INTOXILYZER 8000

Location:

Serial Number : 80-002759

09/23/2010

05:53:45

B4

Standard Lot#: 719919

Last Changed By: C. CONLEY-

#34517

QAS: C. STRAUB

#50772

TUCSON PD

Operator: C. STRAUB

#50772

TUCSON PD

Subject: SQAP, SQAP

DOB: 11/11/1111

Sex: F

Weight: 111

15 Minute Deprivation Period? Yes

Test	g/210L	Time
Air Blank	RFI*	05:54:18
Air Blank	IPS**	05:54:26

*RFI Detect

**Improper Sample

Not a Successfully Completed Test Sequence

Pursuant to section 28-1327, Arizona Revised Statutes, this document is a certified duplicate of the information contained in computer storage devices of the Tucson Police Department.

497
CS

B4

INTOXILYZER 8000

Location:

Serial Number : 80-002759

09/23/2010

05:54:31

Standard Lot#: 719919

Last Changed By: C. CONLEY

#34517

QAS: C. STRAUB

#50772

TUCSON PD

Operator: C. STRAUB

#50772

TUCSON PD

Subject: SQAP, SQAP

DOB: 11/11/1111

Sex: F

Weight: 111

15 Minute Deprivation Period? Yes

Test	g/210L	Time
Air Blank	0.000	05:55:22
Diagnostic Test	Pass	05:55:50
Air Blank	0.000	05:56:17
0.100 Cal Check	0.099	05:56:36
Air Blank	0.000	05:57:05
Subject Test	0.125*	06:00:14
Air Blank	0.000	06:00:46
Air Blank	0.000	06:01:13
Subject Test	XXX**	06:01:43
Air Blank	0.000	06:02:16

*Deficient Sample

**Invalid Sample

Begin new deprivation period

Not a Successfully Completed Test Sequence

587
CS

INTOXILYZER 8000

Location:

Serial Number: 80-002759

09/23/2010

06:02:34

TS4


Standard Lot#: 719919

Last Changed By: C. CONLEY #34517

QAS: C. STRAUB #50772

TUCSON PD

Test	g/210L	Time
Air Blank	0.000	06:03:01
Cal Check	0.097	06:03:20
Air Blank	0.000	06:03:50



Operator's Signature

THIS REPORT PREPARED PURSUANT TO DUTY IMPOSED BY
A.A.C. R13-10-104(A)

ARIZONA DEPARTMENT OF PUBLIC SAFETY

STANDARD QUALITY ASSURANCE PROCEDURES
INTOXILYZER MODEL 8000

STANDARD CALIBRATION CHECK PROCEDURE

By
9.27.2010

QA Specialist Cheryl STRAUB AGENCY Tucson Police Department
DATE 09/23/10 TIME 05:46
Intoxilyzer Serial # 80-002759 Location TEAM 4

- (✓) 1. Ensure that gas tank is attached to instrument and contains a standard alcohol concentration solution 0. 100 AC.
OR
Pour a standard alcohol concentration solution N/A AC, into a clean dry simulator and assemble the simulator. Ensure that a tight seal has been made. Turn on the simulator and allow temperature to reach 34°C ± 0.2°C
- (✓) 2. Intoxilyzer 8000 display reads "PUSH BUTTON TO START"
- (✓) 3. Go to the "Control Testing Menu". Select "D" for dry control test or "W" for wet control test. After selection is made press ENTER.
- (✓) 4. Air blank completed.
- (✓) 5. Calibration check completed. Test results 0. 098 AC.
- (✓) 6. Air blank completed.
- (✓) 7. Remove printed record. Attach the record to the completed checklist.

SIGNATURE

Cheryl Straub

DPS Form Exh G-2 (Rev. 05-01)

707
CS

INTOXILYZER 8000

Location:

Serial Number: 80-002759

09/23/2010

05:46:56

Standard Lot#: 719919


Last Changed By: C. CONLEY #34517

QAS: C. STRAUB #50772

TUCSON PD

by

Test	g/210L	Time
Air Blank	0.000	05:47:23
Cal Check	0.098	05:47:42
Air Blank	0.000	05:48:11



Operator's Signature