



CERTIFICATION by CUSTODIAN of RECORDS
 Tucson Police Department Crime Laboratory
 1306 W. Miracle Mile, Tucson, AZ 85705

T54
 9.27.2011

I hereby certify that these documents are a true and correct copy of the periodic maintenance* for the Intoxilyzer 8000 Serial Number SD - 00 2759 maintained by the Tucson Police Department Crime Laboratory pursuant to the requirements of the Arizona Department of Public Safety for a quality assurance program.

A quality assurance specialist (QAS) tested the instrument on the following dates. The acceptable accuracy limits, as defined in A.A.C. R13-10-104.A.2, for a 0.100AC solution are 0.090AC to 0.110AC.

Date: 9.23-11 Cal 1 0.098 AC Cal 2 0.096 AC

Between the dates of 8.25-11 and 9.23-11 the instrument was operating properly and accurately.

The instrument was taken out of service for repair on N/A.
 The instrument was returned to service on N/A.


Clare Conley

Clare L. Conley

9.23-11

ADPS QAS Permit # 33314

SUBSCRIBED AND SWORN to before me this 23, day of

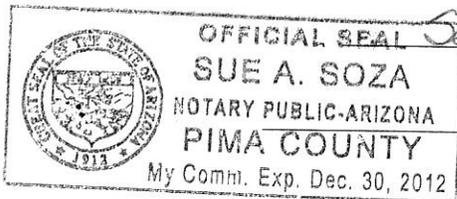

September, 2011.

Sue A. Soza

Notary Public

*Includes documents specified in A.A.C. R13-10-104.A.5

EXHIBIT G-4

THIS REPORT PREPARED PURSUANT TO DUTY IMPOSED BY
A.A.C. R13-10-104(A)

1067
CW

ARIZONA DEPARTMENT OF PUBLIC SAFETY

STANDARD QUALITY ASSURANCE PROCEDURES
INTOXILYZER MODEL 8000

TS4
9.27.2011

STANDARD QUALITY ASSURANCE PROCEDURE

QA SPECIALIST Clare Conley AGENCY Tucson Police Department

DATE 9-23-11 TIME 0710

INTOXILYZER SERIAL # 80-002759 LOCATION ODE

(✓) 1. Display reads "PUSH BUTTON TO START"

DIAGNOSTIC TESTS

(✓) 1. Clock time check.

(✓) 2. Date check.

OPERATIONAL TESTS

(✓) 1. Alcohol-free subject test result 0. 500 AC.

(✓) 2. Error recognition logic system functioning.
Not a Successfully Completed Test Sequence printed

(✓) 3. Proper sample recognition system.
Not a Successfully Completed Test Sequence printed
Deficient sample printed.

(✓) 4. Standard Calibration Check standard 0. 100 AC
Result: 0. 096 AC

Instrument is operating properly and accurately. YES NO

COMMENTS None

SIGNATURE Clare Conley

INTOXILYZER 8000
Location:
Serial Number : 80-002759
09/23/2011

07:12:00

2067
CW

Standard Lot#: 04911100A1
Last Changed By: C. STRAUB #50772

TSG

QAS: C. CONLEY #34517
TUCSON PD

Operator: C. CONLEY #34517
TUCSON PD

Subject: TEST, SQAP

DOB: 11/11/1111

Sex: M

Weight: 111

15 Minute Deprivation Period? Yes

Test	g/210L	Time
Air Blank	0.000	07:12:47
Diagnostic Test	Pass	07:13:15
Air Blank	0.000	07:13:42
0.100 Cal Check	0.097	07:14:01
Air Blank	0.000	07:14:30
Subject Test	0.000	07:14:45
Air Blank	ABT*	07:14:51
Air Blank	0.000	07:15:20

*Sequence Aborted

Not a Successfully Completed Test Sequence

INTOXILYZER 8000
Location:
Serial Number : 80-002759
09/23/2011

07:15:29

367
CM

Standard Lot#: 04911100A1
Last Changed By: C. STRAUB #50772
QAS: C. CONLEY #34517
TUCSON PD

TS4

Operator: C. CONLEY #34517
TUCSON PD

Subject: TEST, SQAP
DOB: 11/11/1111
Sex: M Weight: 111

15 Minute Deprivation Period? Yes

Test	g/210L	Time
Air Blank	RFI*	07:16:01
Air Blank	IPS**	07:16:09

*RFI Detect
**Improper Sample

Not a Successfully Completed Test Sequence

INTOXILYZER 8000
Location:
Serial Number : 80-002759
09/23/2011

07:16:17

4567
CW

Standard Lot#: 04911100A1
Last Changed By: C. STRAUB #50772

BS4

QAS: C. CONLEY #34517
TUCSON PD

Operator: C. CONLEY #34517
TUCSON PD

Subject: TEST,SQAP
DOB: 11/11/1111
Sex: M Weight: 111

15 Minute Deprivation Period? Yes

Test	g/210L	Time
Air Blank	0.000	07:17:21
Diagnostic Test	Pass	07:17:48
Air Blank	0.000	07:18:16
0.100 Cal Check	0.097	07:18:34
Air Blank	0.000	07:19:04
Subject Test	0.109*	07:22:12
Air Blank	0.000	07:22:45
Air Blank	0.000	07:23:12
Subject Test	XXX**	07:23:40
Air Blank	0.000	07:24:14

*Deficient Sample

**Invalid Sample

Begin new deprivation period

Not a Successfully Completed Test Sequence

INTOXILYZER 8000

Location:

Serial Number: 80-002759

09/23/2011

07:24:30

5067
CW

Standard Lot#: 04911100A1


Last Changed By: C. STRAUB #50772

TS4

QAS: C. CONLEY #34517

TUCSON PD

Test	g/210L	Time
Air Blank	0.000	07:24:58
Cal Check	0.096	07:25:17
Air Blank	0.000	07:25:46



Operator's Signature

EXHIBIT G-2

6067
CW

THIS REPORT PREPARED PURSUANT TO DUTY IMPOSED BY
A.A.C. R13-10-104(A)

ARIZONA DEPARTMENT OF PUBLIC SAFETY

STANDARD QUALITY ASSURANCE PROCEDURES
INTOXILYZER MODEL 8000

TS4
9.27.2011

STANDARD CALIBRATION CHECK PROCEDURE

QA Specialist Clare Conley AGENCY Tucson Police Department
DATE 9-23-11 TIME 0710
Intoxilyzer Serial # 80-002759 Location ODE

- (✓) 1. Ensure that gas tank is attached to instrument and contains a standard alcohol concentration solution 0. 100 AC.
OR
Pour a standard alcohol concentration solution _____ AC, into a clean dry simulator and assemble the simulator. Ensure that a tight seal has been made. Turn on the simulator and allow temperature to reach 34°C ± 0.2°C
- (✓) 2. Intoxilyzer 8000 display reads "PUSH BUTTON TO START"
- (✓) 3. Go to the "Control Testing Menu". Select "D" for dry control test or "W" for wet control test. After selection is made press ENTER.
- (✓) 4. Air blank completed.
- (✓) 5. Calibration check completed. Test results 0. 098 AC.
- (✓) 6. Air blank completed.
- (✓) 7. Remove printed record. Attach the record to the completed checklist.

SIGNATURE Clare Conley

DPS Form Exh G-2 (Rev. 05-01)

INTOXILYZER 8000
Location:
Serial Number: 80-002759
09/23/2011 07:10:35

7567
cu
154

Standard Lot#: 04911100A1
Last Changed By: C. STRAUB #50772

QAS: C. CONLEY #34517
TUCSON PD

Test	g/210L	Time
Air Blank	0.000	07:11:03
Cal Check	0.098	07:11:21
Air Blank	0.000	07:11:51

Clare Conley
Operator's Signature