



CERTIFICATION by CUSTODIAN of RECORDS

Tucson Police Department Crime Laboratory
1306 W. Miracle Mile, Tucson, AZ 85705

TS4
3.23.2016

I hereby certify that these documents are a true and correct copy of the periodic maintenance* for the Intoxilyzer 8000 Serial Number 80-002759 maintained by the Tucson Police Department Crime Laboratory pursuant to the requirements of the Arizona Department of Public Safety for a quality assurance program.

A quality assurance specialist (QAS) tested the instrument on the following dates. The acceptable accuracy limits, as defined in A.A.C. R13-10-104.A.2, for a 0.100AC solution are 0.090AC to 0.110AC.

Date: 3/3/2016 Cal 1 0.096 AC Cal 2 0.095 AC

Between the dates of 2/4/2016 and 3/3/2016 the instrument was operating properly and accurately.

The instrument was taken out of service for repair on _____.
The instrument was returned to service on _____.

William L Loomis

William L. Loomis


3/7/2016

ADPS QAS Permit # 33720

SUBSCRIBED AND SWORN to before me this 7th, day of March, 2016.

Elma Escarcega

Notary Public

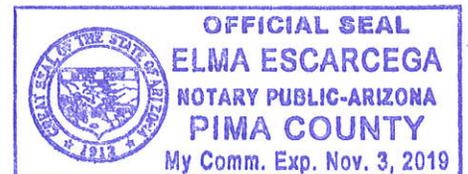

*Includes documents specified in A.A.C. R13-10-104.A.5

EXHIBIT G-4

THIS REPORT PREPARED PURSUANT TO DUTY IMPOSED BY
A.A.C. R13-10-104(A)

ARIZONA DEPARTMENT OF PUBLIC SAFETY
STANDARD QUALITY ASSURANCE PROCEDURES
INTOXILYZER MODEL 8000
STANDARD QUALITY ASSURANCE PROCEDURE

1 of 7
WLL
TJH 3.23.2016

QA SPECIALIST W. LOOMIS 53545 AGENCY Tucson Police Department

DATE 3/3/2016 TIME 09:02

INTOXILYZER SERIAL # 80-002759 LOCATION ODM- SGT'S OFFICE

(✓) 1. Display reads "PUSH BUTTON TO START"

DIAGNOSTIC TESTS

- (✓) 1. Clock time check.
- (✓) 2. Date check.

OPERATIONAL TESTS

- (✓) 1. Alcohol-free subject test result 0. 000 AC.
- (✓) 2. Error recognition logic system functioning.
Not a Successfully Completed Test Sequence printed
- (✓) 3. Proper sample recognition system.
Not a Successfully Completed Test Sequence printed
Deficient sample printed.
- (✓) 4. Standard Calibration Check standard 0. 100 AC
Result: 0. 095 AC

Instrument is operating properly and accurately. YES NO

COMMENTS

SIGNATURE Willie Loomis

Pursuant to section 28-1327, Arizona Revised Statutes, this document is a certified duplicate of the information contained in computer storage devices of the Tucson Police Department.

2 of 7
WU
T54

INTOXILYZER 8000
Location: TUCSON PD
Serial Number: 80-002759
Core Version: 8105.48
03/03/2016 09:05:59

Standard Lot#: 11514100A2
Last Changed By: S. CIONE #50616

OAS: W. LOOMIS #53545
TUCSON PD

Operator: W. LOOMIS #53545
TUCSON PD

Subject: SOAP, SOAP
DOB: 11/11/1987
Sex: M Weight: 222

15 Minute Deprivation Period? Yes

Test	g/210L	Time
Air Blank	0.000	09:06:52
Diagnostic Test	Pass	09:07:29
Air Blank	0.000	09:07:56
0.100 Cal Check	0.095	09:08:17
Air Blank	0.000	09:08:47
Subject Test	0.000	09:09:04
Air Blank	0.000	09:09:32
Wait	ABT*	
Air Blank	0.000	09:10:06

*Sequence Aborted

Not a Successfully
Completed
Test Sequence

3 of 7
WU
T04

INTOXILYZER 8000
Location: TUCSON PD
Serial Number: 80-002759
Core Version: 8105.48
03/03/2016 09:11:40

Standard Lot#: 11514100A2
Last Changed By: S. CIONE #50616

QAS: W. LOOMIS #53545
TUCSON PD

Operator: W. LOOMIS #53545
TUCSON PD

Subject: SOAP, SOAP
DOB: 11/11/1987
Sex: M Weight: 222

15 Minute Deprivation Period? Yes

Test	g/210L	Time
Air Blank	0.000	09:12:32
Diagnostic Test	Pass	09:13:10
Air Blank	0.000	09:13:37
0.100 Cal Check	RFI*	09:13:53
Air Blank	IPS**	09:14:01

*RFI Detect
**Improper Sample

Not a Successfully
Completed
Test Sequence

4 of 7
WLL
TSG

INTOXILYZER 8000
Location: TUCSON PD
Serial Number: 80-002759
Core Version: 8105.48
03/03/2016 09:14:56

Standard Lot#: 11514100A2
Last Changed By: S. CIONE #50616

OAS: W. LOOMIS #53545
TUCSON PD

Operator: W. LOOMIS #53545
TUCSON PD

Subject: SOAP, SOAP
DOB: 11/11/1987
Sex: M Weight: 222

15 Minute Deprivation Period? Yes

Test	g/210L	Time
Air Blank	0.000	09:15:52
Diagnostic Test	Pass	09:16:29
Air Blank	0.000	09:16:57
0.100 Cal Check	0.096	09:17:17
Air Blank	0.000	09:17:47
Subject Test	0.199*	09:20:54
Air Blank	0.000	09:21:27
Air Blank	0.000	09:21:55
Subject Test	XXX**	09:22:18
Air Blank	0.000	09:22:53

*Deficient Sample
**Invalid Sample
Begin new deprivation period

Not a Successfully
Completed
Test Sequence

5 of 7
WU
TSh

INTOXILYZER 8000
Location: TUCSON PD
Serial Number: 80-002759
Core Version: 8105.48
03/13/2016 09:24:15

Standard Lot#: 11514100A2
Last Changed By: S. CIONE #50616

DAS: W. LOOMIS #53545
TUCSON PD

Operator: W. LOOMIS #53545
TUCSON PD

Test	g/210L	Time
Air Blank	0.000	09:24:45
0.100 Cal Check	0.095	09:25:06
Air Blank	0.000	09:25:35

Preventative Maintenance
Performed -- Timer Reset

EXHIBIT G-2

THIS REPORT PREPARED PURSUANT TO DUTY IMPOSED BY
A.A.C. R13-10-104(A)

ARIZONA DEPARTMENT OF PUBLIC SAFETY

STANDARD QUALITY ASSURANCE PROCEDURES
INTOXILYZER MODEL 8000

STANDARD CALIBRATION CHECK PROCEDURE

6 of 7
WU
TSG
3.23.2016

QA Specialist W. LOOMIS 53545 AGENCY Tucson Police Department
DATE 3/3/2016 TIME 09:02
Intoxilyzer Serial # 80-002759 Location ODM - SGT'S OFFICE

- (✓) 1. Ensure that gas tank is attached to instrument and contains a standard alcohol concentration solution 0. 100 AC.
OR
Pour a standard alcohol concentration solution _____ AC, into a clean dry simulator and assemble the simulator. Ensure that a tight seal has been made. Turn on the simulator and allow temperature to reach 34°C ± 0.2°C
- (✓) 2. Intoxilyzer 8000 display reads "PUSH BUTTON TO START"
- (✓) 3. Go to the "Control Testing Menu". Select "D" for dry control test or "W" for wet control test. After selection is made press ENTER.
- (✓) 4. Air blank completed.
- (✓) 5. Calibration check completed. Test results 0. 096 AC.
- (✓) 6. Air blank completed.
- (✓) 7. Remove printed record. Attach the record to the completed checklist.

SIGNATURE Willie Loomis

DPS Form Exh G-2 (Rev. 05-01)

7 of 7
WLL
TS4

INTOXILYZER 8000
Location: TUCSON PD
Serial Number: 80-002759
Core Version: 8105.48
03/03/2016 09:02:40

Standard Lot#: 11514100A2
Last Changed By: S. CIONE #50616

DAS: W. LOOMIS #53545
TUCSON PD

Operator: W. LOOMIS #53545
TUCSON PD

Test	g/210L	Time
Air Blank	0.000	09:03:10
0.100 Cal Check	0.096	09:03:31
Air Blank	0.000	09:04:00

Preventative Maintenance
Performed -- Timer Reset