



CERTIFICATION by CUSTODIAN of RECORDS
Tucson Police Department Crime Laboratory
1306 W. Miracle Mile, Tucson, AZ 85705

TS4
3-23-2016

I hereby certify that these documents are a true and correct copy of the periodic maintenance* for the Intoxilyzer 8000 Serial Number 80-002760 maintained by the Tucson Police Department Crime Laboratory pursuant to the requirements of the Arizona Department of Public Safety for a quality assurance program.

A quality assurance specialist (QAS) tested the instrument on the following dates. The acceptable accuracy limits, as defined in A.A.C. R13-10-104.A.2, for a 0.100AC solution are 0.090AC to 0.110AC.

Date: 3-4-16 Cal 1 0.097 AC Cal 2 0.095 AC

Between the dates of 2-5-16 and 3-4-16 the instrument was operating properly and accurately.

The instrument was taken out of service for repair on .
The instrument was returned to service on .


Amy L. Autret

3-7-16

ADPS QAS Permit # 33718

SUBSCRIBED AND SWORN to before me this 7th, day of March, 2016.

Notary Public

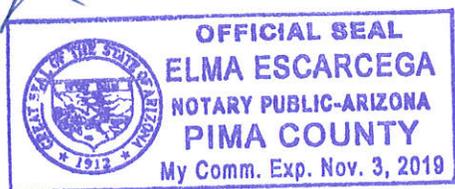

*Includes documents specified in A.A.C. R13-10-104.A.5

EXHIBIT G-4

THIS REPORT PREPARED PURSUANT TO DUTY IMPOSED BY
A.A.C. R13-10-104(A)

ARIZONA DEPARTMENT OF PUBLIC SAFETY
STANDARD QUALITY ASSURANCE PROCEDURES
INTOXILYZER MODEL 8000
STANDARD QUALITY ASSURANCE PROCEDURE

10F7
TS4
3.23.2016

QA SPECIALIST Amy Arct 53546 AGENCY Tucson Police Department

DATE 3-4-16 TIME 0842

INTOXILYZER SERIAL # 80-002760 LOCATION OPE - Intox room

(✓) 1. Display reads "PUSH BUTTON TO START"

DIAGNOSTIC TESTS

(✓) 1. Clock time check.

(✓) 2. Date check.

OPERATIONAL TESTS

(✓) 1. Alcohol-free subject test result 0. 000 AC.

(✓) 2. Error recognition logic system functioning.
Not a Successfully Completed Test Sequence printed


(✓) 3. Proper sample recognition system.
Not a Successfully Completed Test Sequence printed
Deficient sample printed.

(✓) 4. Standard Calibration Check standard 0. 100 AC
Result: 0. 095 AC

Instrument is operating properly and accurately. YES NO

COMMENTS

SIGNATURE

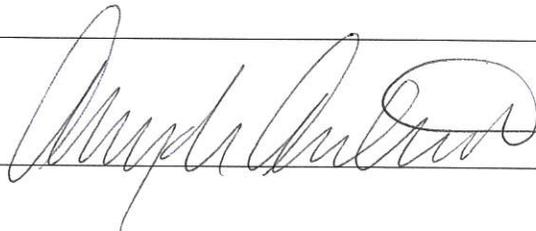

2 of 7
JLS
TS4

INTOXILYZER 8000
Location: TUCSON PD
Serial Number: 80-002760
Core Version: 8105.48
03/04/2016 08:46:49

Standard Lot#: 25414100A4
Last Changed By: T. GALLEGOS #28847

DAS: A. AUTRET #53546
TUCSON PD

Operator: A. AUTRET #53546
TUCSON PD

Subject: SOAP,SOAP
DOB: 11/11/1987
Sex: F Weight: 111

15 Minute Deprivation Period? Yes

Test	g/210L	Time
Air Blank	0.000	08:47:57
Diagnostic Test	Pass	08:48:34
Air Blank	0.000	08:49:02
0.100 Cal Check	0.097	08:49:23
Air Blank	0.000	08:49:52
Subject Test	0.000	08:50:26
Air Blank	0.000	08:50:53
Wait	ABT*	
Air Blank	0.000	08:51:28

*Sequence Aborted

Not a Successfully
Completed
Test Sequence

3 of 7
JLB
B4

INTOXILYZER 8000
Location: TUCSON PD
Serial Number: 80-002760
Core Version: 8105.48
03/04/2016 08:52:28

Standard Lot#: 25414100A4
Last Changed By: T. GALLEGOS #28847

QAS: A. AUTRET #53546
TUCSON PD

Operator: A. AUTRET #53546
TUCSON PD

Subject: SOAP, SOAP
DOB = 11/11/1987
Sex = F Weight: 111

15 Minute Deprivation Period? Yes

Test	g/210L	Time
Air Blank	0.000	08:53:22
Diagnostic Test	Pass	08:53:59
Air Blank	0.000	08:54:27
0.100 Cal Check	RFI*	08:54:39
Air Blank	IPS**	08:54:48

*RFI Detect
**Improper Sample

Not a Successfully
Completed
Test Sequence

4 of 7
Jld
TS4

INTOXILYZER 8000
Location: TUCSON PD
Serial Number: 80-002760
Core Version: 8105.48
03/04/2016 08:55:40

Standard Lot#: 25414100A4
Last Changed By: T. GALLEGOS #28847

DAS: A. AUTRET #53546
TUCSON PD

Operator: A. AUTRET #53546
TUCSON PD

Subject: SOAP_SOAP
DOB: 11/11/1987
Sex: F Weight: 111

15 Minute Deprivation Period? Yes

Test	g/210L	Time
Air Blank	0.000	08:56:37
Diagnostic Test	Pass	08:57:14
Air Blank	0.000	08:57:42
0.100 Cal Check	0.096	08:58:03
Air Blank	0.000	08:58:32
Subject Test	0.078*	09:01:40
Air Blank	0.000	09:02:13
Air Blank	0.000	09:02:41
Subject Test	XXX**	09:03:10
Air Blank	0.000	09:03:44

*Deficient Sample
**Invalid Sample
Begin new deprivation period

Not a Successfully
Completed
Test Sequence

5 of 7
ADD
734

INTOXILYZER 8000
Location: TUCSON PD
Serial Number: 80-002760
Core Version: 8105.48
03/04/2016 09:04:41

Standard Lot#: 25414100A4
Last Changed By: T. GALLEGOS #28847

QAS: A. AUTRET #53546
TUCSON PD

Operator: A. AUTRET #53546
TUCSON PD

Test	g/210L	Time
Air Blank	0.000	09:05:10
0.100 Cal Check	0.095	09:05:31
Air Blank	0.000	09:06:01

Preventative Maintenance
Performed -- Timer Reset

EXHIBIT G-2

THIS REPORT PREPARED PURSUANT TO DUTY IMPOSED BY
A.A.C. R13-10-104(A)

ARIZONA DEPARTMENT OF PUBLIC SAFETY

STANDARD QUALITY ASSURANCE PROCEDURES
INTOXILYZER MODEL 8000

STANDARD CALIBRATION CHECK PROCEDURE

6 of 7
TS4
3.23.2016

QA Specialist Amy Autret 53546 AGENCY Tucson Police Department

DATE 3-4-16 TIME 0842

Intoxilyzer Serial # 80-002760 Location ODE - Intox 100M

- (✓) 1. Ensure that gas tank is attached to instrument and contains a standard alcohol concentration solution 0. 100 AC.
OR
Pour a standard alcohol concentration solution _____ AC, into a clean dry simulator and assemble the simulator. Ensure that a tight seal has been made. Turn on the simulator and allow temperature to reach 34°C ± 0.2°C
- (✓) 2. Intoxilyzer 8000 display reads "PUSH BUTTON TO START"
- (✓) 3. Go to the "Control Testing Menu". Select "D" for dry control test or "W" for wet control test. After selection is made press ENTER.
- (✓) 4. Air blank completed.
- (✓) 5. Calibration check completed. Test results 0. 097 AC.
- (✓) 6. Air blank completed.
- (✓) 7. Remove printed record. Attach the record to the completed checklist.

SIGNATURE



DPS Form Exh G-2 (Rev. 05-01)

7067
JLD
TSH

INTOXILYZER 8000
Instrument Initialization
08:35:41 03/04/2016

INTOXILYZER 8000
Location: TUCSON PD
Serial Number: 80-002760
Core Version: 8105.48
03/04/2016 08:42:48

Standard Lot#: 25414100A4
Last Changed By: T. GALLEGOS #28847

QAS: A. AUTRET #53546
TUCSON PD

Operator: A. AUTRET #53546
TUCSON PD

Test	g/210L	Time
Air Blank	0.000	08:43:19
0.100 Cal Check	0.097	08:43:39
Air Blank	0.000	08:44:09

Preventative Maintenance
Performed -- Timer Reset