



CERTIFICATION by CUSTODIAN of RECORDS

Tucson Police Department Crime Laboratory
1306 W. Miracle Mile, Tucson, AZ 85705

I hereby certify that these documents are a true and correct copy of the periodic maintenance* for the Intoxilyzer 8000 Serial Number 80-006048 maintained by the Tucson Police Department Crime Laboratory pursuant to the requirements of the Arizona Department of Public Safety for a quality assurance program.

TSK
9.29.2014

A quality assurance specialist (QAS) tested the instrument on the following dates. The acceptable accuracy limits, as defined in A.A.C. R13-10-104.A.2, for a 0.100AC solution are 0.090AC to 0.110AC.

Date: 9/11/14 Cal 1 0.097 AC Cal 2 0.097 AC

Between the dates of 8/14/14 and 9/11/14 the instrument was operating properly and accurately.

The instrument was taken out of service for repair on -
The instrument was returned to service on -

Sarah Cione

Sarah L. Cione


9/15/14

ADPS QAS Permit # 33355

SUBSCRIBED AND SWORN to before me this 15th day of September, 2014.

Elma Escarcega

Notary Public

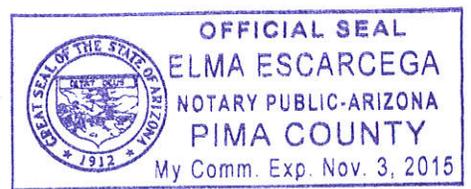

*Includes documents specified in A.A.C. R13-10-104.A.5

EXHIBIT G-4

THIS REPORT PREPARED PURSUANT TO DUTY IMPOSED BY
A.A.C. R13-10-104(A)

ARIZONA DEPARTMENT OF PUBLIC SAFETY

STANDARD QUALITY ASSURANCE PROCEDURES
INTOXILYZER MODEL 8000

STANDARD QUALITY ASSURANCE PROCEDURE

1 of 7
SC
B4
9.29.2014

QA SPECIALIST Sarah Cione AGENCY Tucson Police Department

DATE 9/11/14 TIME 1052

INTOXILYZER SERIAL # 80-006048 LOCATION DUI HQ

(✓) 1. Display reads "PUSH BUTTON TO START"

DIAGNOSTIC TESTS

(✓) 1. Clock time check.

(✓) 2. Date check.

OPERATIONAL TESTS

(✓) 1. Alcohol-free subject test result 0. 000 AC.

(✓) 2. Error recognition logic system functioning.
Not a Successfully Completed Test Sequence printed

(✓) 3. Proper sample recognition system.
Not a Successfully Completed Test Sequence printed
Deficient sample printed.

(✓) 4. Standard Calibration Check standard 0. 100 AC
Result: 0. 097 AC

Instrument is operating properly and accurately. YES NO

COMMENTS

SIGNATURE Sarah Cione

INTOXILYZER 8000
Location: TUCSON PD
Serial Number: 80-006048
Core Version: 8105.48
09/11/2014

10:57:21

2 of 7 sc
TS4

Standard Lot#: 25913100A2
Last Changed By: T. GALLEGOS #28847

QAS: S. CIONE #50616
TUCSON PD

Operator: S. CIONE #50616
TUCSON PD

Subject: SQAP, SQAP
DOB: 11/11/1980
Sex: F Weight: 111

15 Minute Deprivation Period? Yes

Test	g/210L	Time
Air Blank	0.000	10:58:01
Diagnostic Test	Pass	10:58:36
Air Blank	0.000	10:59:04
0.100 Cal Check	0.099	10:59:25
Air Blank	0.000	10:59:54
Subject Test	0.000	11:00:58
Air Blank	0.000	11:01:25
Wait	ABT*	
Air Blank	0.000	11:03:21

*Sequence Aborted

Not a Successfully Completed Test Sequence

INTOXILYZER 8000
Location: TUCSON PD
Serial Number: 80-006048
Core Version: 8105.48
09/11/2014

11:04:22

3 of 7
sc
Tdh

Standard Lot#: 25913100A2
Last Changed By: T. GALLEGOS #28847

QAS: S. CIONE #50616
TUCSON PD

Operator: S. CIONE #50616
TUCSON PD

Subject: SQAP, SQAP
DOB: 11/11/1980
Sex: F Weight: 111

15 Minute Deprivation Period? Yes

Test	g/210L	Time
Air Blank	0.000	11:05:03
Diagnostic Test	Pass	11:05:38
Air Blank	0.000	11:06:05
0.100 Cal Check	0.097	11:06:26
Air Blank	0.000	11:06:56
Subject Test	RFI*	11:07:24
Air Blank	IPS**	11:07:32

*RFI Detect
**Improper Sample

Not a Successfully Completed Test Sequence

Pursuant to section 28-1327, Arizona Revised Statutes, this document is a certified duplicate of the information contained in computer storage devices of the Tucson Police Department.

INTOXILYZER 8000
Location: TUCSON PD
Serial Number: 80-006048
Core Version: 8105.48
09/11/2014

11:08:28

4 of 7
5c
TB4

Standard Lot#: 25913100A2
Last Changed By: T. GALLEGOS #28847

QAS: S. CIONE #50616
TUCSON PD

Operator: S. CIONE #50616
TUCSON PD

Subject: SQAP, SQAP
DOB: 11/11/1980
Sex: F Weight: 111

15 Minute Deprivation Period? Yes

Test	g/210L	Time
Air Blank	0.000	11:09:16
Diagnostic Test	Pass	11:09:51
Air Blank	0.000	11:10:18
0.100 Cal Check	0.097	11:10:39
Air Blank	0.000	11:11:08
Subject Test	0.174*	11:14:16
Air Blank	0.000	11:14:48
Air Blank	0.000	11:15:15
Subject Test	XXX**	11:15:48
Air Blank	0.000	11:16:21

*Deficient Sample

**Invalid Sample

Begin new deprivation period

Not a Successfully Completed Test Sequence

INTOXILYZER 8000
Location: TUCSON PD
Serial Number: 80-006048
Core Version: 8105.48
09/11/2014 11:16:47

Standard Lot#: 25913100A2
Last Changed By: T. GALLEGOS #28847

QAS: S. CIONE #50616
TUCSON PD

Operator: S. CIONE #50616
TUCSON PD

Test	g/210L	Time
Air Blank	0.000	11:17:15
0.100 Cal Check	0.097	11:17:36
Air Blank	0.000	11:18:06

Preventative Maintenance
Performed -- Timer Reset

5 of 7
SC
TSh
9.29.2014

EXHIBIT G-2

THIS REPORT PREPARED PURSUANT TO DUTY IMPOSED BY
A.A.C. R13-10-104(A)

ARIZONA DEPARTMENT OF PUBLIC SAFETY

STANDARD QUALITY ASSURANCE PROCEDURES
INTOXILYZER MODEL 8000

STANDARD CALIBRATION CHECK PROCEDURE

6 of 7
SC
TS4
9.29.2014

QA Specialist Sarah Cione AGENCY Tucson Police Department
DATE 9/11/14 TIME 1052
Intoxilyzer Serial # 80-006048 Location DUT HQ

- (✓) 1. Ensure that gas tank is attached to instrument and contains a standard alcohol concentration solution 0. 100 AC.
OR
Pour a standard alcohol concentration solution _____ AC, into a clean dry simulator and assemble the simulator. Ensure that a tight seal has been made. Turn on the simulator and allow temperature to reach 34°C ± 0.2°C
- (✓) 2. Intoxilyzer 8000 display reads "PUSH BUTTON TO START"
- (✓) 3. Go to the "Control Testing Menu". Select "D" for dry control test or "W" for wet control test. After selection is made press ENTER.
- (✓) 4. Air blank completed.
- (✓) 5. Calibration check completed. Test results 0. 097 AC.
- (✓) 6. Air blank completed.
- (✓) 7. Remove printed record. Attach the record to the completed checklist.

SIGNATURE Sarah Cione

DPS Form Exh G-2 (Rev. 05-01)

Pursuant to section 28-1327, Arizona Revised Statutes, this document is a certified duplicate of the information contained in computer storage devices of the Tucson Police Department.

INTOXILYZER 8000
Location: TUCSON PD
Serial Number: 80-006048
Core Version: 8105.48
09/11/2014 10:52:59

7 of 7
SC
TS4

Standard Lot#: 25913100A2
Last Changed By: T. GALLEGOS #28847

QAS: S. CIONE #50616
TUCSON PD

Operator: S. CIONE #50616
TUCSON PD

Test	g/210L	Time
Air Blank	0.000	10:53:28
0.100 Cal Check	0.097	10:53:49
Air Blank	0.000	10:54:18

Preventative Maintenance
Performed -- Timer Reset