



CERTIFICATION by CUSTODIAN of RECORDS

Tucson Police Department Crime Laboratory  
1306 W. Miracle Mile, Tucson, AZ 85705

TS4  
4-10-2015

I hereby certify that these documents are a true and correct copy of the periodic maintenance\* for the Intoxilyzer 8000 Serial Number 80-006052 maintained by the Tucson Police Department Crime Laboratory pursuant to the requirements of the Arizona Department of Public Safety for a quality assurance program.

A quality assurance specialist (QAS) tested the instrument on the following dates. The acceptable accuracy limits, as defined in A.A.C. R13-10-104.A.2, for a 0.100AC solution are 0.090AC to 0.110AC.

Date: 4/2/2015 Cal 1 0.101 AC Cal 2 0.101 AC

Between the dates of 3/6/2015 and 4/2/2015 the instrument was operating properly and accurately.

The instrument was taken out of service for repair on \_\_\_\_\_.  
The instrument was returned to service on \_\_\_\_\_.

William L Loomis

William L. Loomis


4/2/2015

ADPS QAS Permit # 33720

SUBSCRIBED AND SWORN to before me this 2nd, day of April, 2015.

Elma Escarcega

Notary Public

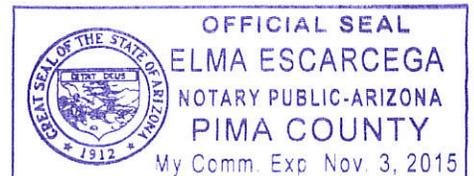

\*Includes documents specified in A.A.C. R13-10-104.A.5

EXHIBIT G-4

THIS REPORT PREPARED PURSUANT TO DUTY IMPOSED BY  
A.A.C. R13-10-104(A)

ARIZONA DEPARTMENT OF PUBLIC SAFETY

STANDARD QUALITY ASSURANCE PROCEDURES  
INTOXILYZER MODEL 8000

STANDARD QUALITY ASSURANCE PROCEDURE

1 of 7  
WLL  
TSh 4.10.2015

QA SPECIALIST W. LOOMIS 53345 AGENCY Tucson Police Department

DATE 4/2/2015 TIME 10:23

INTOXILYZER SERIAL # 80-606052 LOCATION ODE-SGT'S OFFICE

(  ) 1. Display reads "PUSH BUTTON TO START"

DIAGNOSTIC TESTS

- (  ) 1. Clock time check.
- (  ) 2. Date check.

OPERATIONAL TESTS

- (  ) 1. Alcohol-free subject test result 0. 000 AC.
- (  ) 2. Error recognition logic system functioning.  
Not a Successfully Completed Test Sequence printed
- (  ) 3. Proper sample recognition system.  
Not a Successfully Completed Test Sequence printed  
Deficient sample printed.
- (  ) 4. Standard Calibration Check standard 0. 100 AC  
Result: 0. 101 AC

Instrument is operating properly and accurately. YES  NO

COMMENTS

---



---



---



---

SIGNATURE Will Loomis

INTOXILYZER 8000  
Location: TUCSON PD  
Serial Number: 80-006052  
Core Version: 8105.48  
04/02/2015 10:26:01

-----  
Standard Lot#: 25913100A2  
Last Changed By: S. CIONE #50616  
-----

OAS: W. LOOMIS #53545  
TUCSON PD  
-----

Operator: W. LOOMIS #53545  
TUCSON PD  
-----

Subject: SOAP, TEST  
DOB: 11/11/1987  
Sex: M Weight: 222  
-----

15 Minute Deprivation Period? Yes  
-----

Test	g/210L	Time
Air Blank	0.000	10:26:55
Diagnostic Test	Pass	10:27:32
Air Blank	0.000	10:27:59
0.100 Cal Check	0.101	10:28:20
Air Blank	0.000	10:28:50
Subject Test	0.000	10:29:06
Air Blank	0.000	10:29:33
Wait	ABT*	
Air Blank	0.000	10:30:07

\*Sequence Aborted

Not a Successfully  
~~Completed~~  
Test Sequence

2 of 7  
wv  
PS

INTOXILYZER 8000  
Location: TUCSON PD  
Serial Number: 80-006052  
Core Version: 8105.48  
04/02/2015 10:30:35

Standard Lot#: 25913100A2  
Last Changed By: S. CIONE #50616

OAS: W. LOOMIS #53545  
TUCSON PD

Operator: W. LOOMIS #53545  
TUCSON PD

Subject: SOAP, TEST  
DOB: 11/11/1987  
Sex: M Weight: 222

15 Minute Deprivation Period? Yes

Test	g/210L	Time
Air Blank	0.000	10:31:41
Diagnostic Test	Pass	10:32:18
Air Blank	0.000	10:32:46
0.100 Cal Check	RFI*	10:33:01
Air Blank	IPS**	10:33:09

\*RFI Detect  
\*\*Improper Sample

Not a Successfully  
Completed  
~~Test~~ Sequence

3 of 7 WLL  
B4

INTOXILYZER 8000  
Location: TUCSON PD  
Serial Number: 80-006052  
Core Version: 8105.48  
04/02/2015 10:33:46

Standard Lot#: 25913100A2  
Last Changed By: S. CIONE #50616

OAS: W. LOOMIS #53545  
TUCSON PD

Operator: W. LOOMIS #53545  
TUCSON PD

Subject: SOAP, TEST  
DOB: 11/11/1987  
Sex: M Weight: 222

15 Minute Deprivation Period? Yes

Test	g/210L	Time
Air Blank	0.000	10:34:40
Diagnostic Test	Pass	10:35:17
Air Blank	0.000	10:35:44
0.100 Cal Check	0.100	10:36:05
Air Blank	0.000	10:36:35
Subject Test	0.088*	10:39:42
Air Blank	0.000	10:40:16
Air Blank	0.000	10:40:43
Subject Test	XXX**	10:41:02
Air Blank	0.000	10:41:36

\*Deficient Sample  
\*\*Invalid Sample  
Begin new deprivation period

Not a Successfully  
Completed  
Test Sequence

4 of 7 wu

TS4

5 of 7  
WLL  
B4

INTOXILYZER 8000  
Location: TUCSON PD  
Serial Number: 80-006052  
Core Version: 8105.48  
04/02/2015 10:42:22

-----  
Standard Lot#: 25913100A2  
Last Changed By: S. CLONE #50616  
-----

QAS: W. LOOMIS #53545  
TUCSON PD  
-----

Operator: W. LOOMIS #53545  
TUCSON PD  
-----

Test	g/210L	Time
Air Blank	0.000	10:42:53
0.100 Cal Check	0.101	10:43:13
Air Blank	0.000	10:43:43

Preventative Maintenance  
Performed -- Timer Reset

EXHIBIT G-2

THIS REPORT PREPARED PURSUANT TO DUTY IMPOSED BY  
A.A.C. R13-10-104(A)

ARIZONA DEPARTMENT OF PUBLIC SAFETY  
STANDARD QUALITY ASSURANCE PROCEDURES  
INTOXILYZER MODEL 8000  
STANDARD CALIBRATION CHECK PROCEDURE

6 of 7  
WLL  
Bh  
4.10.2015

QA Specialist W. LOOMIS 53545 AGENCY Tucson Police Department  
DATE 4/2/2015 TIME 10:23  
Intoxilyzer Serial # 80-006052 Location ODE - SGT'S OFFICE

- ( ✓ ) 1. Ensure that gas tank is attached to instrument and contains a standard alcohol concentration solution 0. 100 AC.  
OR  
Pour a standard alcohol concentration solution \_\_\_\_\_ AC, into a clean dry simulator and assemble the simulator. Ensure that a tight seal has been made. Turn on the simulator and allow temperature to reach 34°C ± 0.2°C
- ( ✓ ) 2. Intoxilyzer 8000 display reads "PUSH BUTTON TO START"
- ( ✓ ) 3. Go to the "Control Testing Menu". Select "D" for dry control test or "W" for wet control test. After selection is made press ENTER.
- ( ✓ ) 4. Air blank completed.
- ( ✓ ) 5. Calibration check completed. Test results 0. 101 AC.
- ( ✓ ) 6. Air blank completed.
- ( ✓ ) 7. Remove printed record. Attach the record to the completed checklist.

SIGNATURE Will Loomis

Pursuant to section 28-1327, Arizona Revised Statutes, this document is a certified duplicate of the information contained in computer storage devices of the Tucson Police Department.

INTOXILYZER 8000  
Location: TUCSON PD  
Serial Number: 80-006052  
Core Version: 8105.48  
04/02/2015 10:23:30

-----  
Standard Lot#: 25913100A2  
Last Changed By: S. CIONE #50616  
-----

OAS: W. LOOMIS #53545  
TUCSON PD  
-----

Operator: W. LOOMIS #53545  
TUCSON PD  
-----

Test	g/210L	Time
Air Blank	0.000	10:24:01
0.100 Cal Check	0.101	10:24:21
Air Blank	0.000	10:24:51

Preventive Maintenance  
Performed -- Timer Reset

7 of 7  
wll  
TSh