



CERTIFICATION by CUSTODIAN of RECORDS  
Tucson Police Department Crime Laboratory

I hereby certify that these documents are a true and correct copy of the periodic maintenance\* for the Intoxilyzer 5000 Serial Number 64-001226 (#8) maintained by the Tucson Police Department Crime Laboratory pursuant to the requirements of the Arizona Department of Public Safety for a quality assurance program.

A quality assurance specialist (QAS) tested the instrument on the following dates. The acceptable accuracy limits, as defined in A.A.C. R13-10-104.A.2, for a 0.080AC solution are 0.070AC to 0.090AC.

Date: 8-12-06 Cal 1 0.081 AC Cal 2 0.078 AC

Date: 9-8-06 Cal 1 0.080 AC Cal 2 0.079 AC

Date: N/A Cal 1 \_\_\_\_\_ AC Cal 2 \_\_\_\_\_ AC

Between the dates of 8-12-06 and 9-8-06 the instrument was operating properly and accurately.

The instrument was taken out of service for repair on \_\_\_\_\_.  
The instrument was returned to service on \_\_\_\_\_.


Terry S. Gallegos

Terry S. Gallegos

9-12-2006

ADPS QAS Permit # QAS 976

SUBSCRIBED AND SWORN to before me this 12, day of September, 2006.

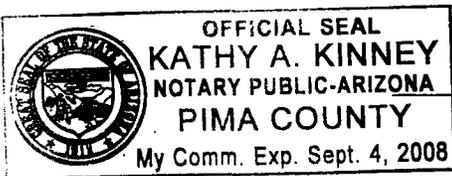

Kathy A Kinney

Notary Public

\*Includes documents specified in A.A.C. R13-10-104.A.5

THIS REPORT PREPARED PURSUANT TO DUTY IMPOSED BY  
A.A.C. R13-10-104(A)

10/6  
TS4

ARIZONA DEPARTMENT OF PUBLIC SAFETY

STANDARD QUALITY ASSURANCE PROCEDURES  
INTOXILYZER MODEL 5000\*

STANDARD QUALITY ASSURANCE PROCEDURE

jk

QA SPECIALIST Terry Gallegos 28847 AGENCY Tucson Police Department  
DATE 9.8.2006 TIME 1629  
INTOXILYZER SERIAL # 64-001226 (#8) LOCATION DUI HQ

( ✓ ) 1. Display reads "READY TO START" or "PUSH BUTTON TO START TEST."

DIAGNOSTIC TESTS

- ( ✓ ) 1. DVM Test check. Setting should be between .010 and .600. Mode selection switch S2 on, S1 and S3 off or keyboard menu selection "H". Reading is .364.
- ( ✓ ) 2. Display Test check. Mode selection switch S1 on and S2 and S3 off or keyboard menu selection "V".
- ( ✓ ) 3. Printer Test check. Mode selection switch S1, S2, S3 off or keyboard menu selection "P".
- ( ✓ ) 4. Clock time check. Mode selection switch S10 on or keyboard menu selection "E".
- ( ✓ ) 5. Date check. Mode selection switch S11 on or keyboard menu selection "E".

OPERATIONAL TESTS

- ( ✓ ) 1. Alcohol-free subject Test result 0. 000 AC
- ( ✓ ) 2. Error recognition logic system functioning  
Invalid test printed
- ( ✓ ) 3. Proper sample recognition system  
Invalid sample printed ✓  
Deficient sample printed ✓
- ( ✓ ) 4. Standard Calibration Check standard 0. 080 AC  
Results: 0. 080AC and 0.079 AC

Instrument operating accurately and properly. YES  NO

COMMENTS:

\_\_\_\_\_  
\_\_\_\_\_  
\_\_\_\_\_

SIGNATURE

Terry Gallegos

\*WITH OR WITHOUT VAPOR RECIRCULATION AND WITH OR WITHOUT KEYBOARD

DPS Form Exh E-4 (Rev. 05-1)

Pursuant to section 28-1327, Arizona Revised Statutes, this document is a certified duplicate of the information contained in computer storage devices of the Tucson Police Department.



# Tucson Police Department Crime Laboratory

3076

D4

gle

FEDERAL SIGNAL CORP. / CMI INC  
 INTOXILYZER - ALCOHOL ANALYZER  
 AZ MODEL 5000 SN 64-001226  
 09/08/06

TEST	BAC VALUE	TIME
AIR BLANK	.000	16:37
CAL. CHECK	.000	16:38
AIR BLANK	.000	16:38

#8

SUBJECT'S NAME

DUI HQ

INSTRUMENT LOCATION

Gallegos 20047

OPERATOR

ADDITIONAL INFORMATION AND/OR REMARKS

TIME FIRST OBSERVED



INTOXILYZER® INSTRUMENT PRINTER CARD

© 1986 by CMI INC.

FEDERAL SIGNAL CORP. / CMI INC  
 INTOXILYZER - ALCOHOL ANALYZER  
 AZ MODEL 5000 SN 64-001226  
 09/08/06

TEST	BAC VALUE	TIME
AIR BLANK	.000	16:39
CAL. CHECK	.079	16:39
AIR BLANK	.000	16:39

#8

SUBJECT'S NAME

DUI HQ

INSTRUMENT LOCATION

Gallegos 20047

OPERATOR

ADDITIONAL INFORMATION AND/OR REMARKS

TIME FIRST OBSERVED



INTOXILYZER® INSTRUMENT PRINTER CARD

© 1986 by CMI INC.

4086  
74  
fle

SN 64-001226  
E47.02  
INVALID TEST  
SAMPLE INTRODUCED  
AT IMPROPER TIME.

09/08/06  
16:54

#8

SUBJECT'S NAME	
DUI HQ	
TIME FIRST OBSERVED	INSTRUMENT LOCATION
Gallegos 25847	
OPERATOR	
ADDITIONAL INFORMATION AND/OR REMARKS	

INTOXILYZER<sup>®</sup> INSTRUMENT PRINTER CARD  
© 1986 by CMI INC.



THIS REPORT PREPARED PURSUANT TO DUTY IMPOSED BY  
A.A.C. R13-10-104(A)

ARIZONA DEPARTMENT OF PUBLIC SAFETY

STANDARD QUALITY ASSURANCE PROCEDURES  
INTOXILYZER MODEL 5000\*

STANDARD CALIBRATION CHECK PROCEDURE

5 of 6  
TSh

QA SPECIALIST Terry Gallegos 28847 AGENCY Tucson Police Department  
DATE 9.8.2006 TIME 1629  
INTOXILYZER SERIAL # 64-001226 (#8) LOCATION DUI HQ

- ( ✓ ) 1. Pour a standard alcohol concentration solution into a clean dry simulator jar and assemble the simulator. Ensure that a tight seal has been made. Standard value: 0. 080 AC.
- ( ✓ ) 2. Turn on the simulator and allow the temperature to reach 34°C ± 0.2°C.
- ( ✓ ) 3. Set Intoxilyzer mode selection in the ACA mode by switching mode selection switch #9 on or selecting "C" on keyboard menu.
- ( ✓ ) 4. Attach simulator to the simulator entrance port on the Intoxilyzer.
- ( ✓ ) 5. Intoxilyzer 5000 display reads "READY TO START" or "PUSH BUTTON".
- ( ✓ ) 6. Push Start Test button or press enter on keyboard.
- ( ✓ ) 7. Insert card in response to display.
- ( ✓ ) 8. Air blank completed.
- ( ✓ ) 9. Standard Calibration Check completed. Test results 0. 080AC and 0.079 AC.
- ( ✓ ) 10. Air blank completed.
- ( ✓ ) 11. When test complete, remove printed record. Attach the record to the completed checklist.
- ( ✓ ) 12. Return mode selection switch #9 to off position after all calibration checks are complete or type Q and enter on keyboard.

SIGNATURE

Terry Gallegos

\*WITH OR WITHOUT VAPOR RECIRCULATION AND WITH OR WITHOUT KEYBOARD

DPS Form Exh E-2 (Rev. 05-1)

FEDERAL SIGNAL CORP. / CMI INC  
INTOXILYZER - ALCOHOL ANALYZER  
AZ MODEL 5000 SN 64-001226  
09/08/06

TEST	BAC VALUE	TIME
AIR BLANK	.000	16:48
INVALID SAMPLE	.XXX	16:49
AIR BLANK	.000	16:49

#8

SUBJECT'S NAME  
DUI HQ

INSTRUMENT LOCATION

TIME FIRST OBSERVED

Gallegos 28847

OPERATOR

ADDITIONAL INFORMATION AND/OR REMARKS

Sweat breath



INTOXILYZER® INSTRUMENT PRINTER CARD

© 1986 by CMI INC.

FEDERAL SIGNAL CORP. / CMI INC  
INTOXILYZER - ALCOHOL ANALYZER  
AZ MODEL 5000 SN 64-001226  
09/08/06

TEST	BAC VALUE	TIME
AIR BLANK	.000	16:50
*SUBJECT TEST	.091	16:52
AIR BLANK	.000	16:53

\* DEFICIENT SAMPLE - VALUE  
PRINTED WAS HIGHEST OBTAINED.

#8

SUBJECT'S NAME  
DUI HQ

INSTRUMENT LOCATION

TIME FIRST OBSERVED

Gallegos 28847

OPERATOR

ADDITIONAL INFORMATION AND/OR REMARKS



INTOXILYZER® INSTRUMENT PRINTER CARD

© 1986 by CMI INC.

6086254 jlc