



CERTIFICATION by CUSTODIAN of RECORDS
Tucson Police Department Crime Laboratory

I hereby certify that these documents are a true and correct copy of the periodic maintenance* for the Intoxilyzer 5000 Serial Number 64-001226 (#8) maintained by the Tucson Police Department Crime Laboratory pursuant to the requirements of the Arizona Department of Public Safety for a quality assurance program.

A quality assurance specialist (QAS) tested the instrument on the following dates. The acceptable accuracy limits, as defined in A.A.C. R13-10-104.A.2, for a 0.080AC solution are 0.070AC to 0.090AC.

Date: 10.6.2006 Cal 1 0.080 AC Cal 2 0.082 AC

Date: 11.3.2006 Cal 1 0.078 AC Cal 2 0.075 AC

Date: — Cal 1 — AC Cal 2 — AC

Between the dates of 10.6.2006 and 11.3.2006 the instrument was operating properly and accurately.

The instrument was taken out of service for repair on N/A.
The instrument was returned to service on N/A.

Terry S. Gallegos


Terry S. Gallegos

12.5.2006

ADPS QAS Permit # QAS 976
SUBSCRIBED AND SWORN to before me this 5th, day of December, 2006.

Rosa Reyna

Notary Public

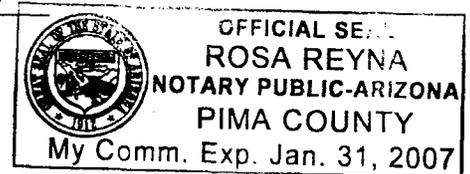

*Includes documents specified in A.A.C. R13-10-104.A.5

1086
B4

THIS REPORT PREPARED PURSUANT TO DUTY IMPOSED BY
A.A.C. R13-10-104(A)

ARIZONA DEPARTMENT OF PUBLIC SAFETY

STANDARD QUALITY ASSURANCE PROCEDURES
INTOXILYZER MODEL 5000*

STANDARD QUALITY ASSURANCE PROCEDURE

QA SPECIALIST Terry Gallegos 28847 AGENCY Tucson Police Department
DATE 11.3.2006 TIME 1504
INTOXILYZER SERIAL # 64-001226 (#8) LOCATION Lub

(✓) 1. Display reads "READY TO START" or "PUSH BUTTON TO START TEST."

DIAGNOSTIC TESTS

- (✓) 1. DVM Test check. Setting should be between .010 and .600. Mode selection switch S2 on, S1 and S3 off or keyboard menu selection "H". Reading is .328.
- (✓) 2. Display Test check. Mode selection switch S1 on and S2 and S3 off or keyboard menu selection "V".
- (✓) 3. Printer Test check. Mode selection switch S1, S2, S3 off or keyboard menu selection "P".
- (✓) 4. Clock time check. Mode selection switch S10 on or keyboard menu selection "E".
- (✓) 5. Date check. Mode selection switch S11 on or keyboard menu selection "E".

OPERATIONAL TESTS

- (✓) 1. Alcohol-free subject Test result 0. 000 AC
- (✓) 2. Error recognition logic system functioning
Invalid test printed
- (✓) 3. Proper sample recognition system
Invalid sample printed ✓
Deficient sample printed ✓
- (✓) 4. Standard Calibration Check standard 0. 080 AC
Results: 0. 078 AC and 0.075 AC

Instrument operating accurately and properly. YES NO

COMMENTS:

SIGNATURE Terry Gallegos

*WITH OR WITHOUT VAPOR RECIRCULATION AND WITH OR WITHOUT KEYBOARD

3096 TS4

Tucson Police Department Crime Laboratory

FEDERAL SIGNAL CORP. / CMI INC
INTOXILYZER - ALCOHOL ANALYZER
AZ MODEL 5000 SN 64-001226
11/03/06

TEST	BAC VALUE	TIME
AIR BLANK	.000	15:15
CAL. CHECK	.078	15:16
AIR BLANK	.000	15:16

#8

SUBJECT'S NAME _____

INSTRUMENT LOCATION Lab

TIME FIRST OBSERVED _____

OPERATOR Gallegos 20047

ADDITIONAL INFORMATION AND/OR REMARKS _____

INTOXILYZER® INSTRUMENT PRINTER CARD

© 1986 by CMI INC.



FEDERAL SIGNAL CORP. / CMI INC
INTOXILYZER - ALCOHOL ANALYZER
AZ MODEL 5000 SN 64-001226
11/03/06

TEST	BAC VALUE	TIME
AIR BLANK	.000	15:17
CAL. CHECK	.075	15:17
AIR BLANK	.000	15:18

#8

SUBJECT'S NAME _____

INSTRUMENT LOCATION Lab

TIME FIRST OBSERVED _____

OPERATOR Gallegos 20047

ADDITIONAL INFORMATION AND/OR REMARKS _____

INTOXILYZER® INSTRUMENT PRINTER CARD

© 1986 by CMI INC.



4 of 6
D4

jk

SN 04-001226 11/03/06
547.02 15:14
INVALID TEST

#8

SUBJECT'S NAME

Lab

TIME FIRST OBSERVED INSTRUMENT LOCATION

Gallenas 28847

OPERATOR

ADDITIONAL INFORMATION AND/OR REMARKS

Pushed start button wrong
time

INTOXILYZER INSTRUMENT PRINTER CARD

EMI INC.

© 1986 by CMI INC.

5086
B4

THIS REPORT PREPARED PURSUANT TO DUTY IMPOSED BY
A.A.C. R13-10-104(A)

ARIZONA DEPARTMENT OF PUBLIC SAFETY

STANDARD QUALITY ASSURANCE PROCEDURES
INTOXILYZER MODEL 5000*

STANDARD CALIBRATION CHECK PROCEDURE

jk

QA SPECIALIST Terry Gallegos 28847 AGENCY Tucson Police Department
DATE 11-3-2006 TIME 1504
INTOXILYZER SERIAL # 64-001226 (#9) LOCATION Lab

- (✓) 1. Pour a standard alcohol concentration solution into a clean dry simulator jar and assemble the simulator. Ensure that a tight seal has been made. Standard value: 0. 080 AC.
- (✓) 2. Turn on the simulator and allow the temperature to reach 34°C ± 0.2°C.
- (✓) 3. Set Intoxilyzer mode selection in the ACA mode by switching mode selection switch #9 on or selecting "C" on keyboard menu.
- (✓) 4. Attach simulator to the simulator entrance port on the Intoxilyzer.
- ✓ 5. Intoxilyzer 5000 display reads "READY TO START" or "PUSH BUTTON".
- ✓ 6. Push Start Test button or press enter on keyboard.
- ✓ 7. Insert card in response to display.
- ✓ 8. Air blank completed.
- ✓ 9. Standard Calibration Check completed. Test results 0. 078AC and 0.075 AC.
- ✓ 10. Air blank completed.
- ✓ 11. When test complete, remove printed record. Attach the record to the completed checklist.
- (✓) 12. Return mode selection switch #9 to off position after all calibration checks are complete or type Q and enter on keyboard.

SIGNATURE *Terry Gallegos*

*WITH OR WITHOUT VAPOR RECIRCULATION AND WITH OR WITHOUT KEYBOARD

DPS Form Exh E-2 (Rev. 05-1)

FEDERAL SIGNAL CORP. / CMI INC
INTOXILYZER - ALCOHOL ANALYZER
AZ MODEL 5000 SN 64-001226
11/03/86

TEST	BAC VALUE	TIME
AIR BLANK	.000	15:05
INVALID SAMPLE	.XXX	15:06
AIR BLANK	.000	15:06

#8

SUBJECT'S NAME

Lab

INSTRUMENT LOCATION

TIME FIRST OBSERVED

Gilkeyos 28847

OPERATOR

ADDITIONAL INFORMATION AND/OR REMARKS

Sweet breath

INTOXILYZER[®] INSTRUMENT PRINTER CARD

© 1986 by CMI INC.



FEDERAL SIGNAL CORP. / CMI INC
INTOXILYZER - ALCOHOL ANALYZER
AZ MODEL 5000 SN 64-001226
11/03/86

TEST	BAC VALUE	TIME
AIR BLANK	.000	15:07
*SUBJECT TEST	.069	15:09
AIR BLANK	.000	15:10

* DEFICIENT SAMPLE - VALUE
PRINTED WAS HIGHEST OBTAINED.

#8

SUBJECT'S NAME

Lab

INSTRUMENT LOCATION

TIME FIRST OBSERVED

Gilkeyos 28847

OPERATOR

ADDITIONAL INFORMATION AND/OR REMARKS

INTOXILYZER[®] INSTRUMENT PRINTER CARD

© 1986 by CMI INC.



6056
D4
He