



CERTIFICATION by CUSTODIAN of RECORDS  
Tucson Police Department Crime Laboratory

*Handwritten initials*

I hereby certify that these documents are a true and correct copy of the periodic maintenance\* for the Intoxilyzer 5000 Serial Number 64-002516 (#12) maintained by the Tucson Police Department Crime Laboratory pursuant to the requirements of the Arizona Department of Public Safety for a quality assurance program.

A quality assurance specialist (QAS) tested the instrument on the following dates. The acceptable accuracy limits, as defined in A.A.C. R9-14-404.A.3, for a 0.080AC solution are 0.070AC to 0.090AC.

Date: 3.16.06 Cal 1 0.075 AC Cal 2 0.074 AC

Date: 4.13.06 Cal 1 0.070 AC Cal 2 0.072 AC

Date: \_\_\_\_\_ Cal 1 \_\_\_\_\_ AC Cal 2 \_\_\_\_\_ AC

Between the dates of 3.16.06 and 4.13.06 the instrument was operating properly and accurately.

The instrument was taken out of service for repair on 4.13.06.

The instrument was returned to service on \_\_\_\_\_.


*Terry S. Gallegos*

Terry S. Gallegos

4.19.2006

ADPS QAS Permit # QAS 976

SUBSCRIBED AND SWORN to before me this 19, day of April, 2006.

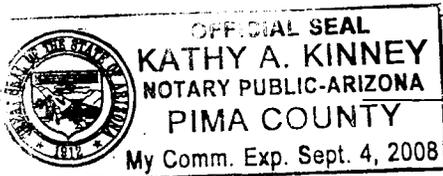

*Kathy A. Kinney*

Notary Public

\*Includes documents specified in A.A.C. R9-14-404.A.6

EXHIBIT Q

1st 6 154

THIS REPORT PREPARED PURSUANT TO DUTY IMPOSED BY  
A.A.C. R9-14-404(A)

ARIZONA DEPARTMENT OF HEALTH SERVICES  
STANDARD QUALITY ASSURANCE PROCEDURES  
INTOXILYZER MODEL 5000\*

AGENCY Tucson Police QA SPECIALIST Terry S. Gallego 28847  
(Print Name)  
INTOXILYZER SERIAL # 64-002516 (#12) LOCATION Traffic  
DATE April 13 18 2006 TIME 1805

Display reads "READY TO START" or "PUSH BUTTON TO START TEST."

DIAGNOSTIC TESTS

- DVM Test check. Setting should be between .200 and .600. Mode selection switch S2 on, S1 and S3 off or keyboard menu selection "H". Reading is .334.
- Display Test check. Mode selection switch S1 on and S2 and S3 off or keyboard menu selection "V".
- Printer Test check. Mode selection switch S1, S2, S3 off or keyboard menu selection "P".
- Clock time check. Mode selection switch S10 on or keyboard menu selection "E".
- Date check. Mode selection switch S11 on or keyboard menu selection "E".

OPERATIONAL TESTS

- Alcohol free subject Test result 0.000 AC
  - Error recognition logic system functioning  
Invalid test printed
  - Proper sample recognition system  
Invalid sample printed ✓  
Deficient sample printed ✓
  - N/A Completeness of sample purge with collection tube\*\*
  - Calibration standard 0.080 AC  
Results: 0.070 AC and 0.072 AC
- Instrument operating properly and accurately. YES  NO

COMMENTS: \_\_\_\_\_  
\_\_\_\_\_

SIGNATURE Terry S. Gallego

0. N/A alcohol concentration standard collected for subsequent analysis.\*\*

\*WITH OR WITHOUT VAPOR RECIRCULATION AND WITH OR WITHOUT KEYBOARD  
\*\*THIS STEP IS ONLY REQUIRED IF THIS DEVICE IS BEING USED FOR  
SAMPLE CAPTURE.



3 of 6  
TSh  
fle

# Tucson Police Department Crime Laboratory

FEDERAL SIGNAL CORP. / CMI INC  
INTOXILYZER - ALCOHOL ANALYZER  
AZ MODEL 5000 SN 64-002516  
04/13/06

| TEST       | BAC VALUE | TIME  |
|------------|-----------|-------|
| AIR BLANK  | .000      | 18:12 |
| CAL. CHECK | .072      | 18:12 |
| AIR BLANK  | .000      | 18:12 |

#12

SUBJECT'S NAME: Traffic

INSTRUMENT LOCATION: \_\_\_\_\_

TIME FIRST OBSERVED: \_\_\_\_\_

OPERATOR: Gallegos 28947

ADDITIONAL INFORMATION AND/OR REMARKS: \_\_\_\_\_



INTOXILYZER INSTRUMENT PRINTER CARD

© 1986 by CMI INC

FEDERAL SIGNAL CORP. / CMI INC  
INTOXILYZER - ALCOHOL ANALYZER  
AZ MODEL 5000 SN 64-002516  
04/13/06

| TEST       | BAC VALUE | TIME  |
|------------|-----------|-------|
| AIR BLANK  | .000      | 18:10 |
| CAL. CHECK | .070      | 18:11 |
| AIR BLANK  | .000      | 18:11 |

#12

SUBJECT'S NAME: Traffic

INSTRUMENT LOCATION: \_\_\_\_\_

TIME FIRST OBSERVED: \_\_\_\_\_

OPERATOR: Gallegos 28847

ADDITIONAL INFORMATION AND/OR REMARKS: \_\_\_\_\_



INTOXILYZER INSTRUMENT PRINTER CARD

© 1986 by CMI INC



EXHIBIT P

506  
B4

THIS REPORT PREPARED PURSUANT TO DUTY IMPOSED BY  
A.A.C. R9-14-404(A)

ARIZONA DEPARTMENT OF HEALTH SERVICES

STANDARD QUALITY ASSURANCE PROCEDURES  
INTOXILYZER MODEL 5000\*

STANDARD CALIBRATION CHECK PROCEDURE

*file*

Agency Tucson Police Department Date 4.13.2006 Time 1805  
Intoxilyzer Serial # 64-002516 (#12) Location Traffic  
QA Specialist Terry S. Gallegos 28847  
(Print Name)

- ( ✓ ) 1. Pour a standard alcohol solution of known value into a clean dry simulator jar and assemble the simulator. Insure that a tight seal has been made. Standard value: 0.080 AC
- ( ✓ ) 2. Turn on the simulator and allow the temperature to reach 34°C + .2°C.
- ( ✓ ) 3. Set Intoxilyzer mode selection in the ACA mode by switching mode selection switch #9 on or selecting "C" on keyboard menu.
- ( ✓ ) 4. Attach simulator to the simulator entrance port on the Intoxilyzer.
- ( ✓ ) 5. Intoxilyzer 5000 display reads "READY TO START" or "PUSH BUTTON".
- ( ✓ ) 6. Push Start Test button or press enter on keyboard.
- ( ✓ ) 7. Insert card in response to display.
- ( ✓ ) 8. Air blank completed.
- ( ✓ ) 9. Calibration check completed. Test results 0.070AC and 0.072 AC
- ( ✓ ) 10. Air blank completed.
- ( ✓ ) 11. When display reads Test Complete remove evidence card. Attach the card to the completed checklist.
- ( ✓ ) 12. Return mode selection switch #9 to off position after all calibration checks are complete or type Q and enter on keyboard.

SIGNATURE Terry S. Gallegos

\*WITH OR WITHOUT VAPOR RECIRCULATION AND WITH OR WITHOUT KEYBOARD

DHS/DSLS/Form C116 (Rev. 7-93)

FEDERAL SIGNAL CORP. / CMI INC  
INTOXILYZER - ALCOHOL ANALYZER  
AZ MODEL 5000 SN 64-002516  
04/13/06

| TEST           | BAC VALUE | TIME  |
|----------------|-----------|-------|
| AIR BLANK      | .000      | 18:20 |
| INVALID SAMPLE | .XXX      | 18:20 |
| AIR BLANK      | .000      | 18:20 |

#12

SUBJECT'S NAME

Traffic

INSTRUMENT LOCATION

TIME FIRST OBSERVED

Gallegos

OPERATOR

ADDITIONAL INFORMATION AND/OR REMARKS

Sweet breath

INTOXILYZER INSTRUMENT PRINTER CARD

© 1986 by CMI INC

**EMI**

FEDERAL SIGNAL CORP. / CMI INC  
INTOXILYZER - ALCOHOL ANALYZER  
AZ MODEL 5000 SN 64-002516  
04/13/06

| TEST          | BAC VALUE | TIME  |
|---------------|-----------|-------|
| AIR BLANK     | .000      | 18:24 |
| *SUBJECT TEST | .072      | 18:23 |
| AIR BLANK     | .000      | 18:24 |

\* DEFICIENT SAMPLE - VALUE  
PRINTED WAS HIGHEST OBTAINED.

#12

SUBJECT'S NAME

Traffic

INSTRUMENT LOCATION

TIME FIRST OBSERVED

Gallegos 28047

OPERATOR

ADDITIONAL INFORMATION AND/OR REMARKS

INTOXILYZER INSTRUMENT PRINTER CARD

© 1986 by CMI INC

**EMI**

0066 T54 file