1 of 6
file

EXHIBIT Q

THIS REPORT PREPARED PURSUANT TO DUTY IMPOSED BY
A.A.C. R9-14-404(A)

ARIZONA DEPARTMENT OF HEALTH SERVICES

STANDARD QUALITY ASSURANCE PROCEDURES 184
INTOXILYZER MODEL 5000*

AGENCY Tucson Police QA SPECIALIST Jennifer Coombs 46160
(Print Name)

INTOXILYZER SERIAL # 66-003327 LOCATION DUI HQ
DATE September 9 ~~18~~ file 2004 TIME 0917

✓ Display reads "READY TO START" or "PUSH BUTTON TO START TEST."

DIAGNOSTIC TESTS

✓ DVM Test check. Setting should be between .200 and .600. Mode selection switch S2 on, S1 and S3 off or keyboard menu selection "H". Reading is .492.

✓ Display Test check. Mode selection switch S1 on and S2 and S3 off or keyboard menu selection "V".

✓ Printer Test check. Mode selection switch S1, S2, S3 off or keyboard menu selection "P".

✓ Clock time check. Mode selection switch S10 on or keyboard menu selection "E".

✓ Date check. Mode selection switch S11 on or keyboard menu selection "E".

OPERATIONAL TESTS

✓ Alcohol free subject Test result 0.000 AC

✓ Error recognition logic system functioning
Invalid test printed

✓ Proper sample recognition system
Invalid sample printed ✓
Deficient sample printed ✓

N/A Completeness of sample purge with collection tube**

✓ Calibration standard 0.080 AC
Results: 0.080AC & 0.079AC

Instrument operating properly and accurately. YES ✓ NO__

COMMENTS: _____

SIGNATURE Jennifer L Coombs

0.N/A alcohol concentration standard collected for subsequent analysis.**

*WITH OR WITHOUT VAPOR RECIRCULATION AND WITH OR WITHOUT KEYBOARD
**THIS STEP IS ONLY REQUIRED IF THIS DEVICE IS BEING USED FOR SAMPLE CAPTURE.

DHS/DSLS/Form C117(Rev.7-93)

SN 66-003327
E767.14 09/09/04
09:25

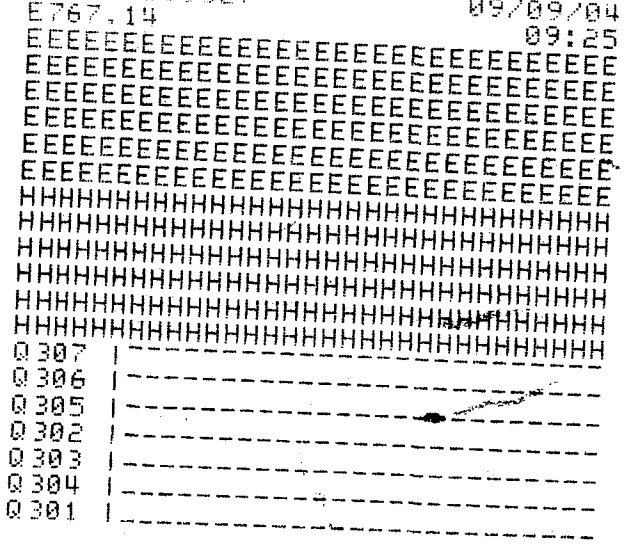

```
EEEEEEEEEEEEEEEEEEEEEEEEEEEEEEEEEEEE
EEEEEEEEEEEEEEEEEEEEEEEEEEEEEEEEEEEE
EEEEEEEEEEEEEEEEEEEEEEEEEEEEEEEEEEEE
EEEEEEEEEEEEEEEEEEEEEEEEEEEEEEEEEEEE
EEEEEEEEEEEEEEEEEEEEEEEEEEEEEEEEEEEE
EEEEEEEEEEEEEEEEEEEEEEEEEEEEEEEEEEEE
HHHHHHHHHHHHHHHHHHHHHHHHHHHHHHHHHHHH
HHHHHHHHHHHHHHHHHHHHHHHHHHHHHHHHHHHH
HHHHHHHHHHHHHHHHHHHHHHHHHHHHHHHHHHHH
HHHHHHHHHHHHHHHHHHHHHHHHHHHHHHHHHHHH
HHHHHHHHHHHHHHHHHHHHHHHHHHHHHHHHHHHH
HHHHHHHHHHHHHHHHHHHHHHHHHHHHHHHHHHHH
Q307 |-----------------------------
Q306 |-----------------------------
Q305 |-----------------------------
Q302 |-----------------------------
Q303 |-----------------------------
Q304 |-----------------------------
Q301 |-----------------------------
```

SUBJECT'S NAME

TIME FIRST OBSERVED

DUI HQ
INSTRUMENT LOCATION

46160
OPERATOR

ADDITIONAL INFORMATION AND/OR REMARKS

INTOXILYZER® INSTRUMENT PRINTER CARD

CMI INC

© 1986 by CMI INC.

TUCSON POLICE DEPARTMENT
INTOXILYZER - ALCOHOL ANALYZER
AZ MODEL 5000 SN 66-003327
09/09/04 09:27

TEST	BRAC VALUE	TIME
AIR BLANK	.000	09:26
SUBJECT TEST	.000	09:26
AIR BLANK	.000	09:27

DVM = .492

SUBJECT'S NAME

TIME FIRST OBSERVED

DUI HQ
INSTRUMENT LOCATION

46160
OPERATOR

ADDITIONAL INFORMATION AND/OR REMARKS

INTOXILYZER® INSTRUMENT PRINTER CARD

CMI INC

© 1986 by CMI INC.

2 of 6

TUCSON POLICE DEPARTMENT
INTOXILYZER - ALCOHOL ANALYZER
AZ MODEL 5000 SN 66-003327
09/09/04 09:29

TEST	BRAC VALUE	TIME
AIR BLANK	.000	09:28
CAL. CHECK	.080	09:29
AIR BLANK	.000	09:29

SUBJECT'S NAME

DUI HQ
INSTRUMENT LOCATION

TIME FIRST OBSERVED

46160
OPERATOR

ADDITIONAL INFORMATION AND/OR REMARKS

INTOXILYZER' INSTRUMENT PRINTER CARD

CMI INC

© 1986 by CMI INC.

TUCSON POLICE DEPARTMENT
INTOXILYZER - ALCOHOL ANALYZER
AZ MODEL 5000 SN 66-003327
09/09/04 09:32

TEST	BRAC VALUE	TIME
AIR BLANK	.000	09:31
CAL. CHECK	.079	09:31
AIR BLANK	.000	09:32

SUBJECT'S NAME

DUI HQ
INSTRUMENT LOCATION

TIME FIRST OBSERVED

46160
OPERATOR

ADDITIONAL INFORMATION AND/OR REMARKS

INTOXILYZER' INSTRUMENT PRINTER CARD

CMI INC

© 1986 by CMI INC.

Tucson Police Department Crime Laboratory

3 of 6

4 of 6
fc

SN 86-003387 09/09/04
E767.14 09:33
INVALID TEST

TEST	BRAC VALUE	TIME
AIR BLANK	.000	09:33

SAMPLE INTRODUCED
AT IMPROPER TIME.

SUBJECT'S NAME

DUI HQ
INSTRUMENT LOCATION

TIME FIRST OBSERVED

461160
OPERATOR

ADDITIONAL INFORMATION AND/OR REMARKS

CMI INC.

INTOXILYZER® INSTRUMENT PRINTER CARD

© 1986 by CMI INC.

5 of 6
jlc

EXHIBIT P

THIS REPORT PREPARED PURSUANT TO DUTY IMPOSED BY
A.A.C. R9-14-404(A)

ARIZONA DEPARTMENT OF HEALTH SERVICES

STANDARD QUALITY ASSURANCE PROCEDURES
INTOXILYZER MODEL 5000*

STANDARD CALIBRATION CHECK PROCEDURE

Agency Tucson Police Department Date 9/9/04 Time 0917
Intoxilyzer Serial# 166-003327 Location DUI HQ
QA Specialist Jennifer Coombs 461160
(Print Name)

(✓) 1. Pour a standard alcohol solution of known value into a clean dry simulator jar and assemble the simulator. Insure that a tight seal has been made.
Standard value: 0.080 AC

(✓) 2. Turn on the simulator and allow the temperature to reach 34°C±.2°C.

(✓) 3. Set Intoxilyzer mode selection in the ACA mode by switching mode selection switch #9 on or selecting "C" on keyboard menu.

(✓) 4. Attach simulator to the simulator entrance port on the Intoxilyzer.

(✓) 5. Intoxilyzer 5000 display reads "READY TO START" or "PUSH BUTTON".

(✓) 6. Push Start Test button or press enter on keyboard.

(✓) 7. Insert card in response to display.

(✓) 8. Air blank completed.

(✓) 9. Calibration check completed.
Test results 0.080AC & 0.079 AC

(✓) 10. Air blank completed.

(✓) 11. When display reads Test Complete remove evidence card. Attach the card to the completed checklist.

(✓) 12. Return mode selection switch #9 to off position after all calibration checks are complete or type Q and enter on keyboard.

SIGNATURE Jennifer L. Coombs

*WITH OR WITHOUT VAPOR RECIRCULATION AND WITH OR WITHOUT KEYBOARD

DHS/DSLS/Form C116 (Rev.7-93)

TUCSON POLICE DEPARTMENT
INTOXILYZER - ALCOHOL ANALYZER
AZ MODEL 5000 SN 66-003327
09/09/04 09:35

TEST	BRAC VALUE	TIME
AIR BLANK	.000	09:34
INVALID SAMPLE	.MOA	09:35
AIR BLANK	.000	09:35

BEGIN NEW DEPRIVATION PERIOD

SUBJECT'S NAME

DUI HQ
INSTRUMENT LOCATION

TIME FIRST OBSERVED

461160
OPERATOR

ADDITIONAL INFORMATION AND/OR REMARKS

Sweet Breath

INTOXILYZER® INSTRUMENT PRINTER CARD

CMI INC

© 1986 by CMI INC.

TUCSON POLICE DEPARTMENT
INTOXILYZER - ALCOHOL ANALYZER
AZ MODEL 5000 SN 66-003327
09/09/04 09:39

TEST	BRAC VALUE	TIME
AIR BLANK	.000	09:36
*SUBJECT TEST	.070	09:39
AIR BLANK	.000	09:39

* DEFICIENT SAMPLE - VALUE PRINTED WAS HIGHEST OBTAINED.

SUBJECT'S NAME

DUI HQ
INSTRUMENT LOCATION

TIME FIRST OBSERVED

461160
OPERATOR

ADDITIONAL INFORMATION AND/OR REMARKS

INTOXILYZER® INSTRUMENT PRINTER CARD

CMI INC

© 1986 by CMI INC.

6 of 6