



CERTIFICATION by CUSTODIAN of RECORDS
Tucson Police Department Crime Laboratory

TS4

I hereby certify that these documents are a true and correct copy of the periodic maintenance* for the Intoxilyzer 5000 Serial Number 66-004798 maintained by the Tucson Police Department Crime Laboratory pursuant to the requirements of the Arizona Department of Public Safety for a quality assurance program.

A quality assurance specialist (QAS) tested the instrument on the following dates. The acceptable accuracy limits, as defined in A.A.C. R13-10-104.A.2, for a 0.080AC solution are 0.070AC to 0.090AC.

Date: 8/3/06 Cal 1 0.078 AC Cal 2 0.078 AC

Date: 9/1/06 Cal 1 0.080 AC Cal 2 0.082 AC

Date: N/A Cal 1 AC Cal 2 AC

Between the dates of 8/3/06 and 9/1/06 the instrument was operating properly and accurately.

The instrument was taken out of service for repair on N/A.


The instrument was returned to service on N/A.

Jennifer L. Coombs
Jennifer L. Coombs

9/8/06

ADPS QAS Permit # QAS 29886

SUBSCRIBED AND SWORN to before me this 8, day of September, 2006.

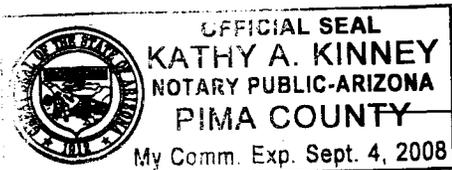

Kathy A Kinney
Notary Public

*Includes documents specified in A.A.C. R13-10-104.A.5

THIS REPORT PREPARED PURSUANT TO DUTY IMPOSED BY
A.A.C. R13-10-104(A)

ARIZONA DEPARTMENT OF PUBLIC SAFETY
STANDARD QUALITY ASSURANCE PROCEDURES
INTOXILYZER MODEL 5000*

1 of 6 file
Tom

STANDARD QUALITY ASSURANCE PROCEDURE

QA SPECIALIST Jennifer Coombs 46160 AGENCY Tucson Police Department
DATE September 1, 2006 TIME 11647
INTOXILYZER SERIAL # 66-004798 LOCATION ODD

() 1. Display reads "READY TO START" or "PUSH BUTTON TO START TEST."

DIAGNOSTIC TESTS

- () 1. DVM Test check. Setting should be between .010 and .600. Mode selection switch S2 on, S1 and S3 off or keyboard menu selection "H". Reading is .365.
- () 2. Display Test check. Mode selection switch S1 on and S2 and S3 off or keyboard menu selection "V".
- () 3. Printer Test check. Mode selection switch S1, S2, S3 off or keyboard menu selection "P".
- () 4. Clock time check. Mode selection switch S10 on or keyboard menu selection "E".
- () 5. Date check. Mode selection switch S11 on or keyboard menu selection "E".

OPERATIONAL TESTS

- () 1. Alcohol-free subject Test result 0. 000 AC
- () 2. Error recognition logic system functioning
Invalid test printed
- () 3. Proper sample recognition system
Invalid sample printed ✓
Deficient sample printed ✓
- () 4. Standard Calibration Check standard 0. 0.080 AC
Results: 0. 0.080 AC # 0.082 AC

Instrument operating accurately and properly. YES NO

COMMENTS:

SIGNATURE Jennifer L. Coombs

*WITH OR WITHOUT VAPOR RECIRCULATION AND WITH OR WITHOUT KEYBOARD

Tucson Police Department Crime Laboratory

3 of 6
file

TUCSON POLICE DEPARTMENT
INTOXILYZER - ALCOHOL ANALYZER
AZ MODEL 5000 SN 66-004798
09/01/06 17:00

TEST BRAC VALUE TIME
AIR BLANK .000 16:59
CAL. CHECK .082 17:00
AIR BLANK .000 17:00

SUBJECT'S NAME

ODD

INSTRUMENT LOCATION

TIME FIRST OBSERVED

46160

OPERATOR

ADDITIONAL INFORMATION AND/OR REMARKS



INTOXILYZER® INSTRUMENT PRINTER CARD

© 1986 by CMI INC.

TUCSON POLICE DEPARTMENT
INTOXILYZER - ALCOHOL ANALYZER
AZ MODEL 5000 SN 66-004798
09/01/06 16:59

TEST BRAC VALUE TIME
AIR BLANK .000 16:58
CAL. CHECK .080 16:58
AIR BLANK .000 16:58

SUBJECT'S NAME

ODD

INSTRUMENT LOCATION

TIME FIRST OBSERVED

46160

OPERATOR

ADDITIONAL INFORMATION AND/OR REMARKS



INTOXILYZER® INSTRUMENT PRINTER CARD

© 1986 by CMI INC.

4 of 6
file

SN 66-004798
E767.14
INVALID TEST

09/01/06
16:50

TEST	BRAC VALUE	TIME
AIR BLANK	.000	16:50

SAMPLE INTRODUCED
AT IMPROPER TIME.

SUBJECT'S NAME

ODD

TIME FIRST OBSERVED

INSTRUMENT LOCATION

46160

OPERATOR

ADDITIONAL INFORMATION AND/OR REMARKS

INTOXILYZER[®] INSTRUMENT PRINTER CARD

EMI_{INC.}

© 1986 by CMI INC.

THIS REPORT PREPARED PURSUANT TO DUTY IMPOSED BY
A.A.C. R13-10-104(A)

ARIZONA DEPARTMENT OF PUBLIC SAFETY
STANDARD QUALITY ASSURANCE PROCEDURES
INTOXILYZER MODEL 5000*

5 of 6
file

STANDARD CALIBRATION CHECK PROCEDURE

QA SPECIALIST Jennifer Coombs 46660 AGENCY Tucson Police Department
DATE September 1, 2006 TIME 1647
INTOXILYZER SERIAL # 166-004798 LOCATION OND

- (✓) 1. Pour a standard alcohol concentration solution into a clean dry simulator jar and assemble the simulator. Ensure that a tight seal has been made. Standard value: 0. 080 AC.
- (✓) 2. Turn on the simulator and allow the temperature to reach 34°C ± 0.2°C.
- (✓) 3. Set Intoxilyzer mode selection in the ACA mode by switching mode selection switch #9 on or selecting "C" on keyboard menu.
- (✓) 4. Attach simulator to the simulator entrance port on the Intoxilyzer.
- ✓✓ 5. Intoxilyzer 5000 display reads "READY TO START" or "PUSH BUTTON".
- ✓✓ 6. Push Start Test button or press enter on keyboard.
- ✓✓ 7. Insert card in response to display.
- ✓✓ 8. Air blank completed.
- ✓✓ 9. Standard Calibration Check completed. Test results 0. 080 AC ± 0.082 AC.
- ✓✓ 10. Air blank completed.
- ✓✓ 11. When test complete, remove printed record. Attach the record to the completed checklist.
- (✓) 12. Return mode selection switch #9 to off position after all calibration checks are complete or type Q and enter on keyboard.

SIGNATURE Jennifer L Coombs

*WITH OR WITHOUT VAPOR RECIRCULATION AND WITH OR WITHOUT KEYBOARD

DPS Form Exh E-2 (Rev. 05-1)

TUCSON POLICE DEPARTMENT
INTOXILYZER - ALCOHOL ANALYZER
AZ MODEL 5000 SN 66-004798
09/01/06 16:52

TEST BRAC VALUE TIME
AIR BLANK .000 16:51
INVALID SAMPLE .MOA 16:51
AIR BLANK .000 16:52

BEGIN NEW DEPRIVATION PERIOD

SUBJECT'S NAME

TIME FIRST OBSERVED

INSTRUMENT LOCATION

46160

OPERATOR

ADDITIONAL INFORMATION AND/OR REMARKS

Sweet Breath

INTOXILYZER INSTRUMENT PRINTER CARD

© 1986 by CMI INC



TUCSON POLICE DEPARTMENT
INTOXILYZER - ALCOHOL ANALYZER
AZ MODEL 5000 SN 66-004798
09/01/06 16:56

TEST BRAC VALUE TIME
AIR BLANK .000 16:53
#SUBJECT TEST .137 16:55
AIR BLANK .000 16:56

* DEFICIENT SAMPLE - VALUE
PRINTED WAS HIGHEST OBTAINED.

SUBJECT'S NAME

TIME FIRST OBSERVED

INSTRUMENT LOCATION

46160

OPERATOR

ADDITIONAL INFORMATION AND/OR REMARKS

INTOXILYZER INSTRUMENT PRINTER CARD

© 1986 by CMI INC



Top 6 of 6 files