1 of 3 pgs
[initials]

EXHIBIT Q

THIS REPORT PREPARED PURSUANT TO DUTY IMPOSED BY
A.A.C. R9-14-404(A)

ARIZONA DEPARTMENT OF HEALTH SERVICES

STANDARD QUALITY ASSURANCE PROCEDURES
INTOXILYZER MODEL 5000*

AGENCY Tucson Police QA SPECIALIST Irene Doran (46331)
(Print Name)

INTOXILYZER SERIAL # 66-004814 LOCATION TRAFFIC
DATE April 14 ~~19~~ 2004 TIME 1014

[initials] Display reads "READY TO START" or "PUSH BUTTON TO START TEST."

DIAGNOSTIC TESTS

[initials] DVM Test check. Setting should be between .200 and .600. Mode selection switch S2 on, S1 and S3 off or keyboard menu selection "H". Reading is .188.

[initials] Display Test check. Mode selection switch S1 on and S2 and S3 off or keyboard menu selection "V".

[initials] Printer Test check. Mode selection switch S1, S2, S3 off or keyboard menu selection "P".

[initials] Clock time check. Mode selection switch S10 on or keyboard menu selection "E".

[initials] Date check. Mode selection switch S11 on or keyboard menu selection "E".

OPERATIONAL TESTS

[initials] Alcohol free subject Test result 0.000 AC

N/A Error recognition logic system functioning
Invalid test printed

N/A Proper sample recognition system
Invalid sample printed
Deficient sample printed

discontinued testing before these would be completed. [initials]

N/A Completeness of sample purge with collection tube**

[initials] Calibration standard 0.080 AC
Results: 0.033 AC + 0.037 AC

Instrument operating properly and accurately. YES__ NO ✓

COMMENTS: * Below DPS range. DVM was unsteady @ .304 + dropped to .188. At this point I stopped DVM testing.

SIGNATURE Irene Doran

0. N/A alcohol concentration standard collected for subsequent analysis.**

*WITH OR WITHOUT VAPOR RECIRCULATION AND WITH OR WITHOUT KEYBOARD
**THIS STEP IS ONLY REQUIRED IF THIS DEVICE IS BEING USED FOR SAMPLE CAPTURE.

** Out of range. Instrument will be sent for service. [initials]

DHS/DSLS/Form C117(Rev.7-93)

SN 66-004814 04/14/04
E767.14 10:21

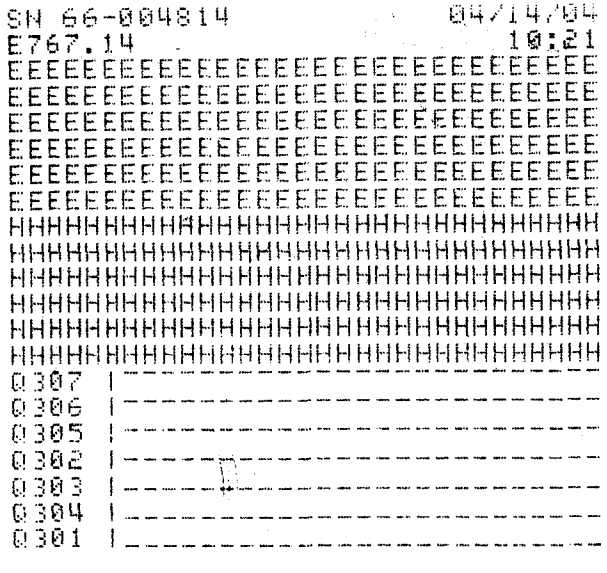


SUBJECT'S NAME

TRAFFIC

TIME FIRST OBSERVED INSTRUMENT LOCATION

DORAN (46331)

OPERATOR

ADDITIONAL INFORMATION AND/OR REMARKS

INTOXILYZER® INSTRUMENT PRINTER CARD

CMI INC

© 1986 by CMI INC.

TUCSON POLICE DEPARTMENT
INTOXILYZER - ALCOHOL ANALYZER
AZ MODEL 5000 SN 66-004814
04/14/04 10:24

| TEST | BRAC VALUE | TIME |
|---|---|---|
| AIR BLANK | .000 | 10:23 |
| SUBJECT TEST | .000 | 10:24 |
| AIR BLANK | .000 | 10:24 |

DVM = .188

SUBJECT'S NAME

TRAFFIC

TIME FIRST OBSERVED INSTRUMENT LOCATION

DORAN (46331)

OPERATOR

ADDITIONAL INFORMATION AND/OR REMARKS

INTOXILYZER® INSTRUMENT PRINTER CARD

CMI INC

© 1986 by CMI INC.

TUCSON POLICE DEPARTMENT
INTOXILYZER - ALCOHOL ANALYZER
AZ MODEL 5000 SN 66-004814
04/14/04 10:26

| TEST | BRAC VALUE | TIME |
|---|---|---|
| AIR BLANK | .000 | 10:25 |
| CAL. CHECK | .033 | 10:26 |
| AIR BLANK | .000 | 10:26 |

SUBJECT'S NAME

TRAFFIC

TIME FIRST OBSERVED INSTRUMENT LOCATION

46331

OPERATOR

ADDITIONAL INFORMATION AND/OR REMARKS

INTOXILYZER® INSTRUMENT PRINTER CARD

CMI INC

© 1986 by CMI INC.

TUCSON POLICE DEPARTMENT
INTOXILYZER - ALCOHOL ANALYZER
AZ MODEL 5000 SN 66-004814
04/14/04 10:28

| TEST | BRAC VALUE | TIME |
|---|---|---|
| AIR BLANK | .000 | 10:28 |
| CAL. CHECK | .037 | 10:28 |
| AIR BLANK | .000 | 10:28 |

SUBJECT'S NAME

TRAFFIC

TIME FIRST OBSERVED INSTRUMENT LOCATION

46331

OPERATOR

ADDITIONAL INFORMATION AND/OR REMARKS

INTOXILYZER® INSTRUMENT PRINTER CARD

CMI INC

© 1986 by CMI INC.

Tucson Police Department Crime Laboratory

3835

4/21/04

585

EXHIBIT P

THIS REPORT PREPARED PURSUANT TO DUTY IMPOSED BY
A.A.C. R9-14-404(A)

ARIZONA DEPARTMENT OF HEALTH SERVICES

STANDARD QUALITY ASSURANCE PROCEDURES
INTOXILYZER MODEL 5000*

STANDARD CALIBRATION CHECK PROCEDURE

Agency Tucson Police Department Date 4/14/04 Time 1014
Intoxilyzer Serial# 66-004814 Location TRAFFIC
QA Specialist Irene Doran (4633)
(Print Name)

1. Pour a standard alcohol solution of known value into a clean dry simulator jar and assemble the simulator. Insure that a tight seal has been made.
   Standard value: 0.080 AC
2. Turn on the simulator and allow the temperature to reach 34°C±.2°C.
3. Set Intoxilyzer mode selection in the ACA mode by switching mode selection switch #9 on or selecting "C" on keyboard menu.
4. Attach simulator to the simulator entrance port on the Intoxilyzer.
5. Intoxilyzer 5000 display reads "READY TO START" or "PUSH BUTTON".
6. Push Start Test button or press enter on keyboard.
7. Insert card in response to display.
8. Air blank completed.
9. Calibration check completed.
   Test results 0.033 + 0.037 AC ☆
10. Air blank completed.
11. When display reads Test Complete remove evidence card. Attach the card to the completed checklist.
12. Return mode selection switch #9 to off position after all calibration checks are complete or type Q and enter on keyboard.

SIGNATURE Irene Doran

*WITH OR WITHOUT VAPOR RECIRCULATION AND WITH OR WITHOUT KEYBOARD

DHS/DSLS/Form C116 (Rev.7-93)

☆ values are out of acceptable range. instrument will be sent out for repair.

4/21/04

182

# TUCSON POLICE DEPARTMENT
# CRIME LABORATORY

## INTOXILYZER SERVICE RECORD

Date: 4/14/04
Intoxilyzer Serial Number: 66-004814
QAS: Irene Doran (46331)

Problem Description:
Simulator solution reading well below target range.

If the instrument is taken out of service, complete the following:

Date out of service 4/14/04

Calibration Check completed prior to removal from service:

☐ Yes Date: _____ ☒ No

SQAP completed prior to removal from service:

☐ Yes Date: _____ ☒ No

Date returned to service: 5/10/04

Corrective Action Taken or Repairs: Blew simulator vapor through breath hose to eliminate simulator as source of problem. Low reading still obtained. Instrument will be sent out for repair

282
95

TUCSON POLICE DEPARTMENT
INTOXILYZER - ALCOHOL ANALYZER
AZ MODEL 5000 SN 66-004814
04/14/04 10:31

| TEST | BRAC VALUE | TIME |
|---|---|---|
| AIR BLANK | .000 | 10:30 |
| SUBJECT TEST | .034 | 10:31 |
| AIR BLANK | .000 | 10:31 |

SUBJECT'S NAME

TIME FIRST OBSERVED

INSTRUMENT LOCATION

OPERATOR

ADDITIONAL INFORMATION AND/OR REMARKS

blowing thru sim. sam.

INTOXILYZER® INSTRUMENT PRINTER CARD

CMI INC

© 1986 by CMI INC.

95