182-110

TUCSON POLICE DEPARTMENT
CRIME LABORATORY

INTOXILYZER SERVICE RECORD

Date: 3/1/04
Intoxilyzer Serial Number: 66-004922
QAS: Irene Doran (46331)

784

Problem Description:
Instrument did not adjust date for leap year.

If the instrument is taken out of service, complete the following:

Date out of service NA

Calibration Check completed prior to removal from service:

☐ Yes Date:_____ ☐ No

SQAP completed prior to removal from service:

☐ Yes Date:_____ ☐ No

Date returned to service: NA

Corrective Action Taken or Repairs:
Adjusted date from 3/2/04 to 3/1/04.

TUCSON POLICE DEPARTMENT
INTOXILYZER - ALCOHOL ANALYZER
AZ MODEL 5000 SN 66-004922
03/02/04 17:46

TEST	BRAC VALUE	TIME
AIR BLANK	.000	17:45
SUBJECT TEST	.000	17:45
AIR BLANK	.000	17:46

SUBJECT'S NAME

TIME FIRST OBSERVED

Team 4 ODE

INSTRUMENT LOCATION

DORAN (46331)

OPERATOR

ADDITIONAL INFORMATION AND/OR REMARKS

Date not changed
w leap year.

INTOXILYZER® INSTRUMENT PRINTER CARD

CMI INC

© 1986 by CMI INC.

ID

TUCSON POLICE DEPARTMENT
INTOXILYZER - ALCOHOL ANALYZER
AZ MODEL 5000 SN 66-004922
03/01/04 17:49

TEST	BRAC VALUE	TIME
AIR BLANK	.000	17:48
SUBJECT TEST	.000	17:49
AIR BLANK	.000	17:49

SUBJECT'S NAME

TIME FIRST OBSERVED

ODE

INSTRUMENT LOCATION

DORAN (46331)

OPERATOR

ADDITIONAL INFORMATION AND/OR REMARKS

Changed date for
leap year.

INTOXILYZER® INSTRUMENT PRINTER CARD

CMI INC

© 1986 by CMI INC.

ID

282

EXHIBIT Q

THIS REPORT PREPARED PURSUANT TO DUTY IMPOSED BY
A.A.C. R9-14-404(A)

ARIZONA DEPARTMENT OF HEALTH SERVICES

STANDARD QUALITY ASSURANCE PROCEDURES
INTOXILYZER MODEL 5000*

AGENCY Tucson Police QA SPECIALIST Irene Doran (46331)
(Print Name)

INTOXILYZER SERIAL # 66-004922 LOCATION ODE
DATE March 14 ~~19~~ 2004 TIME 1316

Display reads "READY TO START" or "PUSH BUTTON TO START TEST."

DIAGNOSTIC TESTS

DVM Test check. Setting should be between .200 and .600. Mode selection switch S2 on, S1 and S3 off or keyboard menu selection "H". Reading is .336.

Display Test check. Mode selection switch S1 on and S2 and S3 off or keyboard menu selection "V".

Printer Test check. Mode selection switch S1, S2, S3 off or keyboard menu selection "P".

Clock time check. Mode selection switch S10 on or keyboard menu selection "E".

Date check. Mode selection switch S11 on or keyboard menu selection "E".

OPERATIONAL TESTS

Alcohol free subject Test result 0.000 AC

Error recognition logic system functioning
Invalid test printed

Proper sample recognition system
Invalid sample printed
Deficient sample printed

N/A Completeness of sample purge with collection tube**

Calibration standard 0.080 AC
Results: 0.077 AC + 0.077 AC

Instrument operating properly and accurately. YES ✓ NO__

COMMENTS: _____

SIGNATURE Irene Doran

0. N/A alcohol concentration standard collected for subsequent analysis.**

*WITH OR WITHOUT VAPOR RECIRCULATION AND WITH OR WITHOUT KEYBOARD
**THIS STEP IS ONLY REQUIRED IF THIS DEVICE IS BEING USED FOR SAMPLE CAPTURE.

DHS/DSLS/Form C117(Rev.7-93)

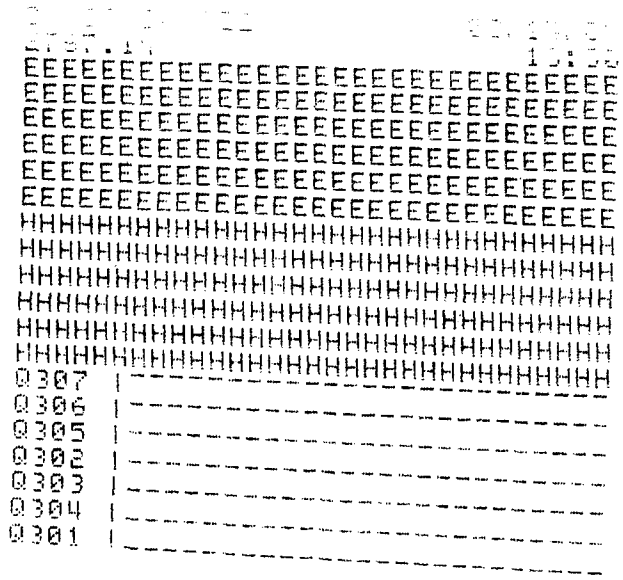

SUBJECT'S NAME

TIME FIRST OBSERVED

INSTRUMENT LOCATION

OPERATOR

ADDITIONAL INFORMATION AND/OR REMARKS

INTOXILYZER® INSTRUMENT PRINTER CARD

CMI INC

© 1986 by CMI INC.

TUCSON POLICE DEPARTMENT
INTOXILYZER - ALCOHOL ANALYZER
AZ MODEL 5000 SN 66-004922
03/14/04 13:17

TEST	BRAC VALUE	TIME
AIR BLANK	.000	13:17
SUBJECT TEST	.000	13:17
AIR BLANK	.000	13:17

DVM= .336

SUBJECT'S NAME

TIME FIRST OBSERVED

INSTRUMENT LOCATION ODE

OPERATOR DORAN (46331)

ADDITIONAL INFORMATION AND/OR REMARKS

INTOXILYZER® INSTRUMENT PRINTER CARD

CMI INC

© 1986 by CMI INC.

TUCSON POLICE DEPARTMENT
INTOXILYZER - ALCOHOL ANALYZER
AZ MODEL 5000 SN 66-004922
03/14/04 13:20

TEST	BRAC VALUE	TIME
AIR BLANK	.000	13:19
CAL. CHECK	.077	13:19
AIR BLANK	.000	13:20

SUBJECT'S NAME

ODE
INSTRUMENT LOCATION

TIME FIRST OBSERVED

DORAN (46331)
OPERATOR

ADDITIONAL INFORMATION AND/OR REMARKS

INTOXILYZER® INSTRUMENT PRINTER CARD

CMI INC

© 1986 by CMI INC.

TUCSON POLICE DEPARTMENT
INTOXILYZER - ALCOHOL ANALYZER
AZ MODEL 5000 SN 66-004922
03/14/04 13:21

TEST	BRAC VALUE	TIME
AIR BLANK	.000	13:21
CAL. CHECK	.077	13:21
AIR BLANK	.000	13:21

SUBJECT'S NAME

ODE
INSTRUMENT LOCATION

TIME FIRST OBSERVED

DORAN (46331)
OPERATOR

ADDITIONAL INFORMATION AND/OR REMARKS

INTOXILYZER® INSTRUMENT PRINTER CARD

CMI INC

© 1986 by CMI INC.

Tucson Police Department Crime Laboratory

4 8 6
PS

SN 86-004922 03/14/04
E767.14 13:33
INVALID TEST

TEST	BRAC VALUE	TIME
AIR BLANK	.000	13:33

PRESSED START TEST AT
IMPROPER TIME

SUBJECT'S NAME

ODE
INSTRUMENT LOCATION

TIME FIRST OBSERVED

DORAN (46331)
OPERATOR

ADDITIONAL INFORMATION AND/OR REMARKS

INTOXILYZER® INSTRUMENT PRINTER CARD

CMI INC.

© 1986 by CMI INC.

PS

3 8 6

EXHIBIT P

THIS REPORT PREPARED PURSUANT TO DUTY IMPOSED BY
A.A.C. R9-14-404(A)

ARIZONA DEPARTMENT OF HEALTH SERVICES

STANDARD QUALITY ASSURANCE PROCEDURES
INTOXILYZER MODEL 5000*

STANDARD CALIBRATION CHECK PROCEDURE

Agency Tucson Police Department Date 3/14/04 Time 1316
Intoxilyzer Serial# 66-04922 Location ODE
QA Specialist Irene Doran (46331)
(Print Name)

(✓) 1. Pour a standard alcohol solution of known value into a clean dry simulator jar and assemble the simulator. Insure that a tight seal has been made.
Standard value: 0.080 AC

(✓) 2. Turn on the simulator and allow the temperature to reach 34°C±.2°C.

(✓) 3. Set Intoxilyzer mode selection in the ACA mode by switching mode selection switch #9 on or selecting "C" on keyboard menu.

(✓) 4. Attach simulator to the simulator entrance port on the Intoxilyzer.

(✓) 5. Intoxilyzer 5000 display reads "READY TO START" or "PUSH BUTTON".

(✓) 6. Push Start Test button or press enter on keyboard.

(✓) 7. Insert card in response to display.

(✓) 8. Air blank completed.

(✓) 9. Calibration check completed.
Test results 0.077 + 0.077 AC

(✓) 10. Air blank completed.

(✓) 11. When display reads Test Complete remove evidence card. Attach the card to the completed checklist.

(✓) 12. Return mode selection switch #9 to off position after all calibration checks are complete or type Q and enter on keyboard.

SIGNATURE Irene Doran

*WITH OR WITHOUT VAPOR RECIRCULATION AND WITH OR WITHOUT KEYBOARD

DHS/DSLS/Form C116 (Rev.7-93)

TUCSON POLICE DEPARTMENT
INTOXILYZER - ALCOHOL ANALYZER
AZ MODEL 5000 SN 66-004922
03/14/04 13:32

TEST	BRAC VALUE	TIME
AIR BLANK	.000	13:32
INVALID SAMPLE	.MOA	13:32
AIR BLANK	.000	13:32

BEGIN NEW DEPRIVATION PERIOD

SUBJECT'S NAME

TIME FIRST OBSERVED

ODE
INSTRUMENT LOCATION

DORAN 46331
OPERATOR

ADDITIONAL INFORMATION AND/OR REMARKS

Binaca

INTOXILYZER® INSTRUMENT PRINTER CARD

CMI INC

© 1986 by CMI INC.

TUCSON POLICE DEPARTMENT
INTOXILYZER - ALCOHOL ANALYZER
AZ MODEL 5000 SN 66-004922
03/14/04 13:25

TEST	BRAC VALUE	TIME
AIR BLANK	.000	13:22
*SUBJECT TEST	.076	13:25
AIR BLANK	.000	13:25

* DEFICIENT SAMPLE - VALUE PRINTED WAS HIGHEST OBTAINED.

SUBJECT'S NAME

TIME FIRST OBSERVED

ODE
INSTRUMENT LOCATION

DORAN (46331)
OPERATOR

ADDITIONAL INFORMATION AND/OR REMARKS

INTOXILYZER® INSTRUMENT PRINTER CARD

CMI INC

© 1986 by CMI INC.