1 of 1

# TUCSON POLICE DEPARTMENT
# CRIME LABORATORY

## INTOXILYZER SERVICE RECORD

Date: 2/9/04
Intoxilyzer Serial Number: 66-005003
QAS: Irene Doran (46331)

Problem Description:
2/9/04 Officer Barrett reported the Intox Date as erroneous (Oct 37 2004) and time incorrect

If the instrument is taken out of service, complete the following:

Date out of service N/A

Calibration Check completed prior to removal from service:

☐ Yes Date:_____ ☐ No

SQAP completed prior to removal from service:

☐ Yes Date:_____ ☐ No

Date returned to service: N/A

Corrective Action Taken or Repairs:
Adjusted date + time. Officer Noting correct time + date.

EXHIBIT Q

THIS REPORT PREPARED PURSUANT TO DUTY IMPOSED BY
A.A.C. R9-14-404(A)

ARIZONA DEPARTMENT OF HEALTH SERVICES

STANDARD QUALITY ASSURANCE PROCEDURES
INTOXILYZER MODEL 5000*

AGENCY Tucson Police QA SPECIALIST Irene Doran (46331)
(Print Name)

INTOXILYZER SERIAL #66-005003 LOCATION DUI HQ
DATE February 25 ~~19~~ 2004 TIME 1000
95

95 Display reads "READY TO START" or "PUSH BUTTON TO START TEST."

DIAGNOSTIC TESTS

95 DVM Test check. Setting should be between .200 and .600. Mode selection switch S2 on, S1 and S3 off or keyboard menu selection "H". Reading is .367.

95 Display Test check. Mode selection switch S1 on and S2 and S3 off or keyboard menu selection "V".

95* Printer Test check. Mode selection switch S1, S2, S3 off or keyboard menu selection "P".

95 Clock time check. Mode selection switch S10 on or keyboard menu selection "E".

95 Date check. Mode selection switch S11 on or keyboard menu selection "E".

OPERATIONAL TESTS

95 Alcohol free subject Test result 0.000 AC

95 Error recognition logic system functioning
Invalid test printed

95 Proper sample recognition system
Invalid sample printed
Deficient sample printed 95

N/A Completeness of sample purge with collection tube**

95 Calibration standard 0.080 AC
Results: 0.076AC & 0.077AC

Instrument operating properly and accurately. YES ✓ NO__

COMMENTS: * Characters bouncing up to Left. Cleaned printer rollers. Repeated printer diagnostic and Alcohol free subject test.

SIGNATURE Irene Doran

0. N/A 95 alcohol concentration standard collected for subsequent analysis.**

*WITH OR WITHOUT VAPOR RECIRCULATION AND WITH OR WITHOUT KEYBOARD
**THIS STEP IS ONLY REQUIRED IF THIS DEVICE IS BEING USED FOR SAMPLE CAPTURE.

DHS/DSLS/Form C117(Rev.7-93)

SN 66 005003 02/25/04
E767.14 12:52

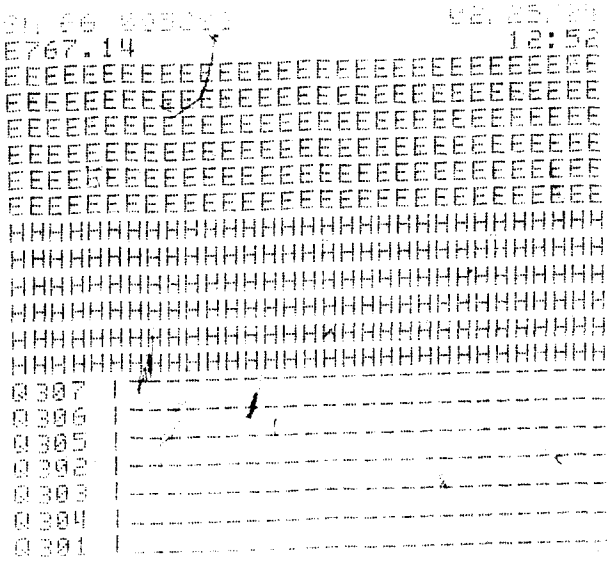


SUBJECT'S NAME

DUI HQ
INSTRUMENT LOCATION

TIME FIRST OBSERVED

DORAN (46331)
OPERATOR

ADDITIONAL INFORMATION AND/OR REMARKS

after printer rollers cleaned

INTOXILYZER® INSTRUMENT PRINTER CARD

CMI INC

© 1986 by CMI INC.

CMI INC
INTOXILYZER - ALCOHOL ANALYZER
AZ MODEL 5000 SN 66-005003
02/25/04 13:07

| TEST | BRAC VALUE | TIME |
|---|---|---|
| AIR BLANK | .000 | 13:06 |
| SUBJECT TEST | .000 | 13:07 |
| AIR BLANK | .000 | 13:07 |

DVM = .367

SUBJECT'S NAME

DUI HQ
INSTRUMENT LOCATION

TIME FIRST OBSERVED

DORAN (46331)
OPERATOR

ADDITIONAL INFORMATION AND/OR REMARKS

after printer roller cleaned

INTOXILYZER® INSTRUMENT PRINTER CARD

CMI INC

© 1986 by CMI INC.

SN 66-005001 02/25/04
E767.14 12:52
EEEEEEEEEEEEEEEEEEEEEEEEEEEEEEEEE
EEEEEEEEEEEEEEEEEEEEEEEEEEEEEEEEE
EEEEEEEEEEEEEEEEEEEEEEEEEEEEEEEEE
EEEEEEEEEEEEEEEEEEEEEEEEEEEEEEEEE
EEEEEEEEEEEEEEEEEEEEEEEEEEEEEEEEE
EEEEEEEEEEEEEEEEEEEEEEEEEEEEEEEEE
HHHHHHHHHHHHHHHHHHHHHHHHHHHHHHHH
HHHHHHHHHHHHHHHHHHHHHHHHHHHHHHHH
HHHHHHHHHHHHHHHHHHHHHHHHHHHHHHHH
HHHHHHHHHHHHHHHHHHHHHHHHHHHHHHHH
HHHHHHHHHHHHHHHHHHHHHHHHHHHHHHHH
HHHHHHHHHHHHHHHHHHHHHHHHHHHHHHHH
Q307 |
Q306 |
Q305 |
Q302 |
Q303 |
Q304 |
Q301 |

SUBJECT'S NAME

DUI HQ
INSTRUMENT LOCATION

TIME FIRST OBSERVED

DORAN (46331)
OPERATOR

ADDITIONAL INFORMATION AND/OR REMARKS

after printer rollers cleaned

INTOXILYZER® INSTRUMENT PRINTER CARD

CMI INC

© 1986 by CMI INC.

CMI INC
INTOXILYZER - ALCOHOL ANALYZER
AI MODEL 5000 SN 66-005003
02/25/04 13:07

| TEST | BRAC VALUE | TIME |
|---|---|---|
| AIR BLANK | .000 | 13:06 |
| SUBJECT TEST | .000 | 13:07 |
| AIR BLANK | .000 | 13:07 |

DVM = .367

SUBJECT'S NAME

DUI HQ
INSTRUMENT LOCATION

TIME FIRST OBSERVED

DORAN (46331)
OPERATOR

ADDITIONAL INFORMATION AND/OR REMARKS

after printer roller cleaned

INTOXILYZER® INSTRUMENT PRINTER CARD

CMI INC

© 1986 by CMI INC.

286

CMI INC
INTOXILYZER - ALCOHOL ANALYZER
AZ MODEL 5000 SN 66-005003
02/25/04 12:59

| TEST | BRAC VALUE | TIME |
|---|---|---|
| AIR BLANK | .000 | 12:58 |
| CAL. CHECK | .076 | 12:59 |
| AIR BLANK | .000 | 12:59 |

SUBJECT'S NAME

TIME FIRST OBSERVED

DUI HQ
INSTRUMENT LOCATION

DORAN (46331)
OPERATOR

ADDITIONAL INFORMATION AND/OR REMARKS

INTOXILYZER® INSTRUMENT PRINTER CARD

© 1986 by CMI INC.

CMI INC
INTOXILYZER - ALCOHOL ANALYZER
AZ MODEL 5000 SN 66-005003
02/25/04 13:00

| TEST | BRAC VALUE | TIME |
|---|---|---|
| AIR BLANK | .000 | 13:00 |
| CAL. CHECK | .077 | 13:00 |
| AIR BLANK | .000 | 13:00 |

SUBJECT'S NAME

TIME FIRST OBSERVED

DUI HQ
INSTRUMENT LOCATION

DORAN (46331)
OPERATOR

ADDITIONAL INFORMATION AND/OR REMARKS

INTOXILYZER® INSTRUMENT PRINTER CARD

© 1986 by CMI INC.

Tucson Police Department Crime Laboratory

486

INVALID TEST

PRESSED START TEST AT
IMPROPER TIME

SUBJECT'S NAME

DUI HQ

TIME FIRST OBSERVED

INSTRUMENT LOCATION

DORTAN (46331)

OPERATOR

ADDITIONAL INFORMATION AND/OR REMARKS

INTOXILYZER® INSTRUMENT PRINTER CARD

CMI INC

© 1986 by CMI INC.

B 86

EXHIBIT P

THIS REPORT PREPARED PURSUANT TO DUTY IMPOSED BY
A.A.C. R9-14-404(A)

ARIZONA DEPARTMENT OF HEALTH SERVICES

STANDARD QUALITY ASSURANCE PROCEDURES
INTOXILYZER MODEL 5000*

STANDARD CALIBRATION CHECK PROCEDURE

Agency Tucson Police Department Date 2/25/04 Time 1000
Intoxilyzer Serial# 66-005003 Location DUI HQ
QA Specialist Irene Doran (46331)
(Print Name)

1. Pour a standard alcohol solution of known value into a clean dry simulator jar and assemble the simulator. Insure that a tight seal has been made.
   Standard value: 0.080 AC
2. Turn on the simulator and allow the temperature to reach 34°C±.2°C.
3. Set Intoxilyzer mode selection in the ACA mode by switching mode selection switch #9 on or selecting "C" on keyboard menu.
4. Attach simulator to the simulator entrance port on the Intoxilyzer.
5. Intoxilyzer 5000 display reads "READY TO START" or "PUSH BUTTON".
6. Push Start Test button or press enter on keyboard.
7. Insert card in response to display.
8. Air blank completed.
9. Calibration check completed.
   Test results 0.076 & 0.077 AC
10. Air blank completed.
11. When display reads Test Complete remove evidence card. Attach the card to the completed checklist.
12. Return mode selection switch #9 to off position after all calibration checks are complete or type Q and enter on keyboard.

SIGNATURE Irene Doran

*WITH OR WITHOUT VAPOR RECIRCULATION AND WITH OR WITHOUT KEYBOARD

DHS/DSLS/Form C116 (Rev.7-93)

CMI INC
INTOXILYZER - ALCOHOL ANALYZER
AZ MODEL 5000 SN 66-005003
02/25/04 13:20

| TEST | BRAC VALUE | TIME |
|---|---|---|
| AIR BLANK | .000 | 13:20 |
| INVALID SAMPLE | .MOA | 13:20 |
| AIR BLANK | .000 | 13:20 |

BEGIN NEW DEPRIVATION PERIOD

SUBJECT'S NAME

DUI HQ

TIME FIRST OBSERVED INSTRUMENT LOCATION

DORAN (46331)

OPERATOR

ADDITIONAL INFORMATION AND/OR REMARKS

Binaca

INTOXILYZER® INSTRUMENT PRINTER CARD

CMI INC

© 1986 by CMI INC.

CMI INC
INTOXILYZER - ALCOHOL ANALYZER
AZ MODEL 5000 SN 66-005003
02/25/04 13:06

| TEST | BRAC VALUE | TIME |
|---|---|---|
| AIR BLANK | .000 | 13:02 |
| *SUBJECT TEST | .071 | 13:05 |
| AIR BLANK | .000 | 13:05 |

* DEFICIENT SAMPLE - VALUE PRINTED WAS HIGHEST OBTAINED.

SUBJECT'S NAME

DUI HQ

TIME FIRST OBSERVED INSTRUMENT LOCATION

DORAN (46331)

OPERATOR

ADDITIONAL INFORMATION AND/OR REMARKS

INTOXILYZER® INSTRUMENT PRINTER CARD

CMI INC

© 1986 by CMI INC.

6 36
69

183
005

# TUCSON POLICE DEPARTMENT
# CRIME LABORATORY

## INTOXILYZER SERVICE RECORD

Date: 2/25/04
Intoxilyzer Serial Number: 66-005003
QAS: Irene Doran (46331)

Problem Description:
Characters bunching up on left side during printer diagnostic + Alcohol free subject test

If the instrument is taken out of service, complete the following:

Date out of service N/A

Calibration Check completed prior to removal from service:

☐ Yes Date:_____ ☐ No

SQAP completed prior to removal from service:

☐ Yes Date:_____ ☐ No

Date returned to service: N/A

Corrective Action Taken or Repairs:
Cleaned printer roller. Repeated printer diagnostic and Alcohol free subject test.

E767.14 10:09

#5003

Q07
Q06
Q05
Q02
Q03
Q04
Q01

SUBJECT'S NAME

TIME FIRST OBSERVED

DUI #Q

INSTRUMENT LOCATION

DORAN (46331)

OPERATOR

ADDITIONAL INFORMATION AND/OR REMARKS

INTOXILYZER® INSTRUMENT PRINTER CARD

CMI INC

© 1986 by CMI INC.

3.05 003003 02/25/04

E767.14 12:52

Q307
Q306
Q305
Q302
Q303
Q304
Q301

SUBJECT'S NAME

TIME FIRST OBSERVED

DUI HQ

INSTRUMENT LOCATION

DORAN (46331)

OPERATOR

ADDITIONAL INFORMATION AND/OR REMARKS

after printer rollers cleaned

INTOXILYZER® INSTRUMENT PRINTER CARD

CMI INC

© 1986 by CMI INC.

233

CMI INC
INTOXILYZER -ALCOHOL ANALYZER
AZ MDEL 5000 SN 66-005003
02/2/0 10:06

| TEST | BRAC VALUE | TIME |
|---|---|---|
| AI BANI | .000 | 10:05 |
| SUJET EST | .000 | 10:06 |
| AF BANI | .000 | 10:06 |

SUBJECT'S NAME

TIME FIRST OBSERVED

INSTRUMENT LOCATION

OPERATOR

ADDITIONAL INFORMATION AND/OR REMARKS

INTOXILYZER® INSTRUMENT PRINTER CARD

CMI INC

© 1986 by CMI INC.

95

CMI INC
INTOXILYZER - ALCOHOL ANALYZER
AZ MODEL 5000 SN 66-005003
02/25/04 13:07

| TEST | BRAC VALUE | TIME |
|---|---|---|
| AIR BLANK | .000 | 13:06 |
| SUBJECT TEST | .000 | 13:07 |
| AIR BLANK | .000 | 13:07 |

DVM = 0367

SUBJECT'S NAME

TIME FIRST OBSERVED

INSTRUMENT LOCATION

OPERATOR

ADDITIONAL INFORMATION AND/OR REMARKS

After panic button cleared

INTOXILYZER® INSTRUMENT PRINTER CARD

CMI INC

© 1986 by CMI INC.

95

Tucson Police Department Crime Laboratory

383
95