



CERTIFICATION by CUSTODIAN of RECORDS
Tucson Police Department Crime Laboratory

I hereby certify that these documents are a true and correct copy of the periodic maintenance* for the Intoxilyzer 5000 Serial Number 66-005003 maintained by the Tucson Police Department Crime Laboratory pursuant to the requirements of the Arizona Department of Public Safety for a quality assurance program.

A quality assurance specialist (QAS) tested the instrument on the following dates. The acceptable accuracy limits, as defined in A.A.C. R9-14-404.A.3, for a 0.080AC solution are 0.070AC to 0.090AC.

Date: 3.16.06 Cal 1 0.078 AC Cal 2 0.079 AC

Date: 4.13.06 Cal 1 0.075 AC Cal 2 0.076 AC

Date: _____ Cal 1 _____ AC Cal 2 _____ AC

Between the dates of 3.16.06 and 4.13.06 the instrument was operating properly and accurately.

The instrument was taken out of service for repair on _____.
The instrument was returned to service on _____.


Terry S. Gallegos

Terry S. Gallegos

4.19.2006

ADPS QAS Permit # QAS 976

SUBSCRIBED AND SWORN to before me this 19, day of April, 2006.

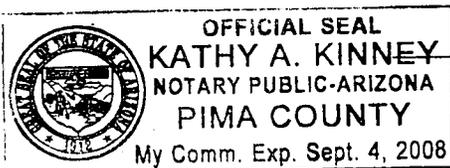

Kathy A. Kinney

Notary Public

*Includes documents specified in A.A.C. R9-14-404.A.6

1 of 6
TS4

THIS REPORT PREPARED PURSUANT TO DUTY IMPOSED BY
A.A.C. R9-14-404(A)

ARIZONA DEPARTMENT OF HEALTH SERVICES
STANDARD QUALITY ASSURANCE PROCEDURES
INTOXILYZER MODEL 5000*

AGENCY Tucson Police QA SPECIALIST Terry S. Gallegos 28847
(Print Name)

INTOXILYZER SERIAL # 66-005003 LOCATION ODW
DATE April 13 ¹⁸/_{B4} 2006 TIME 1508

Display reads "READY TO START" or "PUSH BUTTON TO START TEST."

DIAGNOSTIC TESTS

- DVM Test check. Setting should be between .200 and .600. Mode selection switch S2 on, S1 and S3 off or keyboard menu selection "H". Reading is .358.
- Display Test check. Mode selection switch S1 on and S2 and S3 off or keyboard menu selection "V".
- Printer Test check. Mode selection switch S1, S2, S3 off or keyboard menu selection "P".
- Clock time check. Mode selection switch S10 on or keyboard menu selection "E".
- Date check. Mode selection switch S11 on or keyboard menu selection "E".

OPERATIONAL TESTS

- Alcohol free subject Test result 0.000 AC
- Error recognition logic system functioning
Invalid test printed
- Proper sample recognition system
Invalid sample printed ✓
Deficient sample printed ✓
- N/A Completeness of sample purge with collection tube**
- Calibration standard 0.080 AC
Results: 0.075AC and 0.076AC
- Instrument operating properly and accurately. YES NO

COMMENTS: _____

SIGNATURE _____

0. N/A alcohol concentration standard collected for subsequent analysis.**

*WITH OR WITHOUT VAPOR RECIRCULATION AND WITH OR WITHOUT KEYBOARD
**THIS STEP IS ONLY REQUIRED IF THIS DEVICE IS BEING USED FOR
SAMPLE CAPTURE.

3056 T&G

Tucson Police Department Crime Laboratory

file

TUCSON POLICE DEPARTMENT
INTOXILYZER ALCOHOL ANALYZER
AZ MODEL 5000 SN 66-005603
04/13/86 15:20

TEST SPEC VALUE TIME
AIR BLANK .000 15:19
CAL. CHECK .075 15:19
AIR BLANK .000 15:19

SUBJECT'S NAME _____

TIME FIRST OBSERVED _____ INSTRUMENT LOCATION **ODW**

OPERATOR **Gallegos 28847**

ADDITIONAL INFORMATION AND/OR REMARKS _____

INTOXILYZER INSTRUMENT PRINTER CARD
© 1986 by GMI INC.

INTOXILYZER INSTRUMENT PRINTER CARD
© 1986 by GMI INC.

TUCSON POLICE DEPARTMENT
INTOXILYZER ALCOHOL ANALYZER
AZ MODEL 5000 SN 66-005603
04/13/86 15:19

TEST SPEC VALUE TIME
AIR BLANK .000 15:17
CAL. CHECK .075 15:18
AIR BLANK .000 15:18

SUBJECT'S NAME _____

TIME FIRST OBSERVED _____ INSTRUMENT LOCATION **ODW**

OPERATOR **Gallegos 28847**

ADDITIONAL INFORMATION AND/OR REMARKS _____

4 of 6
Pg

file

SN 66-085003	04/13/06	
E767.14	15:17	
INVALID TEST		
TEST	BRAC VALUE	TIME
AIR BLANK	.000	15:16
PRESSED START TEST AT IMPROPER TIME		
ODW		
SUBJECT'S NAME		
ODW		
TIME FIRST OBSERVED	INSTRUMENT LOCATION	
Gallegos 28847		
OPERATOR		
ADDITIONAL INFORMATION AND/OR REMARKS		
INTOXILYZER [®] INSTRUMENT PRINTER CARD		
		
© 1986 by CMI INC.		

EXHIBIT P

506
124

THIS REPORT PREPARED PURSUANT TO DUTY IMPOSED BY
A.A.C. R9-14-404(A)

ARIZONA DEPARTMENT OF HEALTH SERVICES

STANDARD QUALITY ASSURANCE PROCEDURES
INTOXILYZER MODEL 5000*

STANDARD CALIBRATION CHECK PROCEDURE

Agency Tucson Police Department Date 4.13.2006 Time 1508
Intoxilyzer Serial # 66-005003 Location ODW
QA Specialist Terry S. Gallegos 28847
(Print Name)

- (✓) 1. Pour a standard alcohol solution of known value into a clean dry simulator jar and assemble the simulator. Insure that a tight seal has been made. Standard value: 0.080 AC
- (✓) 2. Turn on the simulator and allow the temperature to reach 34°C ± .2°C.
- (✓) 3. Set Intoxilyzer mode selection in the ACA mode by switching mode selection switch #9 on or selecting "C" on keyboard menu.
- (✓) 4. Attach simulator to the simulator entrance port on the Intoxilyzer.
- (✓✓) 5. Intoxilyzer 5000 display reads "READY TO START" or "PUSH BUTTON".
- (✓✓) 6. Push Start Test button or press enter on keyboard.
- (✓✓) 7. Insert card in response to display.
- (✓✓) 8. Air blank completed.
- (✓✓) 9. Calibration check completed. Test results 0.075AC and 0.076 AC
- (✓✓) 10. Air blank completed.
- (✓✓) 11. When display reads Test Complete remove evidence card. Attach the card to the completed checklist.
- (✓) 12. Return mode selection switch #9 to off position after all calibration checks are complete or type Q and enter on keyboard.

SIGNATURE

Terry S. Gallegos

*WITH OR WITHOUT VAPOR RECIRCULATION AND WITH OR WITHOUT KEYBOARD

DHS/DSLS/Form C116 (Rev. 7-93)

TUCSON POLICE DEPARTMENT
INTOXILYZER - ALCOHOL ANALYZER
AZ MODEL 5000 SN 66-005003
04/13/86 15:10

TEST BRAC VALUE TIME
AIR BLANK .000 15:10
INVALID SAMPLE :NDA 15:10
AIR BLANK .000 15:10

BEGIN NEW DEPRIVATION PERIOD
* DEFICIENT SAMPLE - VALUE
PRINTED WAS HIGHEST OBTAINED.

SUBJECT'S NAME _____
INSTRUMENT LOCATION _____
TIME FIRST OBSERVED _____
OPERATOR Gallegos 28847
ADDITIONAL INFORMATION AND/OR REMARKS _____



INTOXILYZER* INSTRUMENT PRINTER CARD

© 1986 by CMI INC

6086 ISM
JL

TUCSON POLICE DEPARTMENT
INTOXILYZER - ALCOHOL ANALYZER
AZ MODEL 5000 SN 66-005003
04/13/86 15:10

TEST BRAC VALUE TIME
AIR BLANK .000 15:10
INVALID SAMPLE :NDA 15:10
AIR BLANK .000 15:10

BEGIN NEW DEPRIVATION PERIOD

SUBJECT'S NAME _____
INSTRUMENT LOCATION _____
TIME FIRST OBSERVED _____
OPERATOR Gallegos 28847
ADDITIONAL INFORMATION AND/OR REMARKS Sweet breath



INTOXILYZER* INSTRUMENT PRINTER CARD

© 1986 by CMI INC