



CERTIFICATION by CUSTODIAN of RECORDS
Tucson Police Department Crime Laboratory

TS4

I hereby certify that these documents are a true and correct copy of the periodic maintenance* for the Intoxilyzer 5000 Serial Number 166-005003 maintained by the Tucson Police Department Crime Laboratory pursuant to the requirements of the Arizona Department of Public Safety for a quality assurance program.

A quality assurance specialist (QAS) tested the instrument on the following dates. The acceptable accuracy limits, as defined in A.A.C. R13-10-104.A.2, for a 0.080AC solution are 0.070AC to 0.090AC.

Date: 8/3/06 Cal 1 0.075 AC Cal 2 0.077 AC

Date: 9/1/06 Cal 1 0.079 AC Cal 2 0.078 AC

Date: N/A Cal 1 AC Cal 2 AC

Between the dates of 8/3/06 and 9/1/06 the instrument was operating properly and accurately.


The instrument was taken out of service for repair on N/A.
The instrument was returned to service on N/A.

Jennifer L. Coombs
Jennifer L. Coombs

9/12/06

ADPS QAS Permit # QAS 29886

SUBSCRIBED AND SWORN to before me this 12, day of September, 2006.

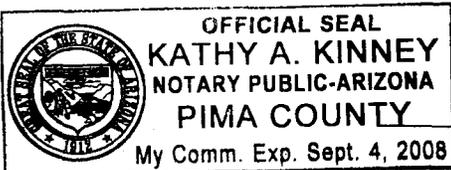

Kathy A. Kinney
Notary Public

*Includes documents specified in A.A.C. R13-10-104.A.5

THIS REPORT PREPARED PURSUANT TO DUTY IMPOSED BY
A.A.C. R13-10-104(A)

ARIZONA DEPARTMENT OF PUBLIC SAFETY

STANDARD QUALITY ASSURANCE PROCEDURES
INTOXILYZER MODEL 5000*

STANDARD QUALITY ASSURANCE PROCEDURE

1 of 6
file

PS

QA SPECIALIST Jennifer Coombs 46160 AGENCY Tucson Police Department
DATE September 1, 2006 TIME 1016
INTOXILYZER SERIAL # 66-005003 LOCATION ODW

() 1. Display reads "READY TO START" or "PUSH BUTTON TO START TEST."

DIAGNOSTIC TESTS

- () 1. DVM Test check. Setting should be between .010 and .600. Mode selection switch S2 on, S1 and S3 off or keyboard menu selection "H". Reading is 342.
- () 2. Display Test check. Mode selection switch S1 on and S2 and S3 off or keyboard menu selection "V".
- () 3. Printer Test check. Mode selection switch S1, S2, S3 off or keyboard menu selection "P".
- () 4. Clock time check. Mode selection switch S10 on or keyboard menu selection "E".
- () 5. Date check. Mode selection switch S11 on or keyboard menu selection "E".

OPERATIONAL TESTS

- () 1. Alcohol-free subject Test result 0. 000 AC
- () 2. Error recognition logic system functioning
Invalid test printed
- () 3. Proper sample recognition system
Invalid sample printed ✓
Deficient sample printed ✓
- () 4. Standard Calibration Check standard 0. 080 AC
Results: 0. 079AC & 0. 078 AC

Instrument operating accurately and properly. YES NO

COMMENTS: * moved clock 1011 → 1016

SIGNATURE Jennifer L. Coombs

*WITH OR WITHOUT VAPOR RECIRCULATION AND WITH OR WITHOUT KEYBOARD

DPS Form Exh E-4 (Rev. 05-1)

Pursuant to section 28-1327, Arizona Revised Statutes, this document is a certified duplicate of the information contained in computer storage devices of the Tucson Police Department.

Tucson Police Department Crime Laboratory

3 of 6
file

TUCSON POLICE DEPARTMENT
INTOXILYZER - ALCOHOL ANALYZER
AZ MODEL 5000 SN 66-005003
09/01/06 10:26

TEST BRAC VALUE TIME
AIR BLANK .000 10:26
CAL. CHECK .078 10:26
AIR BLANK .000 10:26

SUBJECT'S NAME

ASW

INSTRUMENT LOCATION

TIME FIRST OBSERVED

46160

OPERATOR

ADDITIONAL INFORMATION AND/OR REMARKS



INTOXILYZER[®] INSTRUMENT PRINTER CARD

© 1986 by CMI INC.

TUCSON POLICE DEPARTMENT
INTOXILYZER - ALCOHOL ANALYZER
AZ MODEL 5000 SN 66-005003
09/01/06 10:25

TEST BRAC VALUE TIME
AIR BLANK .000 10:24
CAL. CHECK .079 10:25
AIR BLANK .000 10:25

SUBJECT'S NAME

ASW

INSTRUMENT LOCATION

TIME FIRST OBSERVED

46160

OPERATOR

ADDITIONAL INFORMATION AND/OR REMARKS



INTOXILYZER[®] INSTRUMENT PRINTER CARD

© 1986 by CMI INC.

4 of 6
AS ju

SN 66-005003 06/01/06
E767.14 10:21
INVALID TEST

TEST	BRAC VALUE	TIME
AIR BLANK	.000	10:21

SAMPLE INTRODUCED
AT IMPROPER TIME.

SUBJECT'S NAME

OSW

TIME FIRST OBSERVED INSTRUMENT LOCATION

46160

OPERATOR

ADDITIONAL INFORMATION AND /OR REMARKS

INTOXILYZER[®] INSTRUMENT PRINTER CARD



© 1986 by CMI INC.

THIS REPORT PREPARED PURSUANT TO DUTY IMPOSED BY
A.A.C. R13-10-104(A)

ARIZONA DEPARTMENT OF PUBLIC SAFETY

STANDARD QUALITY ASSURANCE PROCEDURES
INTOXILYZER MODEL 5000*

5 of 6
jlc

STANDARD CALIBRATION CHECK PROCEDURE

QA SPECIALIST Jennifer Coombs 46160 AGENCY Tucson Police Department
DATE September 1, 2006 TIME 10/6
INTOXILYZER SERIAL # 66-005003 LOCATION ODW

- (✓) 1. Pour a standard alcohol concentration solution into a clean dry simulator jar and assemble the simulator. Ensure that a tight seal has been made. Standard value: 0. 080 AC.
- (✓) 2. Turn on the simulator and allow the temperature to reach 34°C ± 0.2°C.
- (✓) 3. Set Intoxilyzer mode selection in the ACA mode by switching mode selection switch #9 on or selecting "C" on keyboard menu.
- (✓) 4. Attach simulator to the simulator entrance port on the Intoxilyzer.
- ✓ 5. Intoxilyzer 5000 display reads "READY TO START" or "PUSH BUTTON".
- ✓ 6. Push Start Test button or press enter on keyboard.
- ✓ 7. Insert card in response to display.
- ✓ 8. Air blank completed.
- ✓ 9. Standard Calibration Check completed. Test results 0. 079 AC ± 0.078 AC.
- ✓ 10. Air blank completed.
- ✓ 11. When test complete, remove printed record. Attach the record to the completed checklist.
- (✓) 12. Return mode selection switch #9 to off position after all calibration checks are complete or type Q and enter on keyboard.

SIGNATURE Jennifer L. Coombs

*WITH OR WITHOUT VAPOR RECIRCULATION AND WITH OR WITHOUT KEYBOARD

DPS Form Exh E-2 (Rev. 05-1)

TUCSON POLICE DEPARTMENT
INTOXILYZER - ALCOHOL ANALYZER
AZ MODEL 5000 SN 66-005003
09/01/06 10:32

TEST BRAC VALUE TIME
AIR BLANK .000 10:29
*SUBJECT TEST .160 10:32
AIR BLANK .000 10:32

* DEFICIENT SAMPLE - VALUE
PRINTED WAS HIGHEST OBTAINED.

SUBJECT'S NAME

ODW

INSTRUMENT LOCATION

TIME FIRST OBSERVED

Holloo

OPERATOR

ADDITIONAL INFORMATION AND/OR REMARKS



INTOXILYZER INSTRUMENT PRINTER CARD

© 1986 by CMI INC.

TUCSON POLICE DEPARTMENT
INTOXILYZER - ALCOHOL ANALYZER
AZ MODEL 5000 SN 66-005003
09/01/06 10:28

TEST BRAC VALUE TIME
AIR BLANK .000 10:28
INVALID SAMPLE .NDA 10:28
AIR BLANK .000 10:28

BEGIN NEW DEPRIVATION PERIOD

SUBJECT'S NAME

ODW

INSTRUMENT LOCATION

TIME FIRST OBSERVED

Holloo

OPERATOR

ADDITIONAL INFORMATION AND/OR REMARKS

Sweet Breath



INTOXILYZER INSTRUMENT PRINTER CARD

© 1986 by CMI INC.

6 of 6
file