



CERTIFICATION by CUSTODIAN of RECORDS
Tucson Police Department Crime Laboratory

BN

I hereby certify that these documents are a true and correct copy of the periodic maintenance* for the Intoxilyzer 5000 Serial Number 166-005005 maintained by the Tucson Police Department Crime Laboratory pursuant to the requirements of the Arizona Department of Public Safety for a quality assurance program.

A quality assurance specialist (QAS) tested the instrument on the following dates. The acceptable accuracy limits, as defined in A.A.C. R9-14-404.A.3, for a 0.080AC solution are 0.070AC to 0.090AC.

Date: 2/23/06 Cal 1 0.076 AC Cal 2 0.076 AC

Date: 3/23/06 Cal 1 0.080 AC Cal 2 0.080 AC

Date: N/A Cal 1 AC Cal 2 AC

Between the dates of 2/23/06 and 3/23/06 the instrument was operating properly and accurately.


The instrument was taken out of service for repair on N/A.
The instrument was returned to service on N/A.

Jennifer L. Coombs
Jennifer L. Coombs

3/31/06

ADPS QAS Permit # QAS 29886

SUBSCRIBED AND SWORN to before me this 31, day of March, 2006.

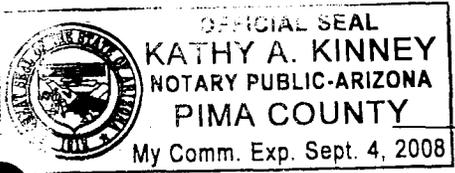

Kathy A. Kinney
Notary Public

*Includes documents specified in A.A.C. R9-14-404.A.6

EXHIBIT Q

1 of 6
file

THIS REPORT PREPARED PURSUANT TO DUTY IMPOSED BY
A.A.C. R9-14-404(A)

ARIZONA DEPARTMENT OF HEALTH SERVICES

STANDARD QUALITY ASSURANCE PROCEDURES
INTOXILYZER MODEL 5000*

134

AGENCY Tucson Police QA SPECIALIST Jennifer Coombs 46160
(Print Name)

INTOXILYZER SERIAL # 66-005705 LOCATION DUI HQ
DATE March 23 19 2006 TIME 1549

Display reads "READY TO START" or "PUSH BUTTON TO START TEST."

DIAGNOSTIC TESTS

- DVM Test check. Setting should be between .200 and .600. Mode selection switch S2 on, S1 and S3 off or keyboard menu selection "H". Reading is .529.
- Display Test check. Mode selection switch S1 on and S2 and S3 off or keyboard menu selection "V".
- Printer Test check. Mode selection switch S1, S2, S3 off or keyboard menu selection "P".
- Clock time check. Mode selection switch S10 on or keyboard menu selection "E".
- Date check. Mode selection switch S11 on or keyboard menu selection "E".

OPERATIONAL TESTS

- Alcohol free subject Test result 0.000 AC
 - Error recognition logic system functioning
Invalid test printed
 - Proper sample recognition system
Invalid sample printed
Deficient sample printed
 - N/A Completeness of sample purge with collection tube**
 - Calibration standard 0.050 AC
Results: 0.050 AC & 0.050 AC
- Instrument operating properly and accurately. YES NO

COMMENTS: _____

SIGNATURE Jennifer L. Coombs

0. N/A alcohol concentration standard collected for subsequent analysis.**

*WITH OR WITHOUT VAPOR RECIRCULATION AND WITH OR WITHOUT KEYBOARD
**THIS STEP IS ONLY REQUIRED IF THIS DEVICE IS BEING USED FOR
SAMPLE CAPTURE.

DHS/DSLS/Form C117 (Rev. 7-93)

Pursuant to section 28-1327, Arizona Revised Statutes, this document is a certified duplicate of the information contained in computer storage devices of the Tucson Police Department.

Tucson Police Department Crime Laboratory *54*

3 of 6 files

TUCSON POLICE DEPARTMENT
INTOXILYZER - ALCOHOL ANALYZER
AZ MODEL 5000 SN 66-905095
03/23/06 16:05

TEST BRAC VALUE TIME
AIR BLANK .000 16:05
CAL. CHECK .000 16:05
AIR BLANK .000 16:05

SUBJECT'S NAME

TIME FIRST OBSERVED

INSTRUMENT LOCATION
DULT HQ

OPERATOR
Hollo
ADDITIONAL INFORMATION AND/OR REMARKS



INTOXILYZER INSTRUMENT PRINTER CARD
© 1986 by CMI, INC.

TUCSON POLICE DEPARTMENT
INTOXILYZER - ALCOHOL ANALYZER
AZ MODEL 5000 SN 66-905095
03/23/06 16:04

TEST BRAC VALUE TIME
AIR BLANK .000 16:03
CAL. CHECK .000 16:03
AIR BLANK .000 16:04

SUBJECT'S NAME

TIME FIRST OBSERVED

INSTRUMENT LOCATION
DULT HQ

OPERATOR
Hollo
ADDITIONAL INFORMATION AND/OR REMARKS



INTOXILYZER INSTRUMENT PRINTER CARD
© 1986 by CMI, INC.

4 of 6
JH JH

SN 66-005003
E767.14
INVALID TEST

03/23/06
16:02

SAMPLE INTRODUCED
AT IMPROPER TIME.

SUBJECT'S NAME

TIME FIRST OBSERVED
DUI HQ
INSTRUMENT LOCATION

46160
OPERATOR

ADDITIONAL INFORMATION AND/OR REMARKS

INTOXILYZER[®] INSTRUMENT PRINTER CARD
© 1986 by CMI INC



EXHIBIT P

5 of 6
file

THIS REPORT PREPARED PURSUANT TO DUTY IMPOSED BY
A.A.C. R9-14-404(A)

ARIZONA DEPARTMENT OF HEALTH SERVICES
STANDARD QUALITY ASSURANCE PROCEDURES
INTOXILYZER MODEL 5000*

104

STANDARD CALIBRATION CHECK PROCEDURE

Agency Tucson Police Department Date 3/23/06 Time 1549
Intoxilyzer Serial # 66-05005 Location DUI HQ
QA Specialist Jennifer Coombs 461100
(Print Name)

- (✓) 1. Pour a standard alcohol solution of known value into a clean dry simulator jar and assemble the simulator. Insure that a tight seal has been made. Standard value: 0.080 AC
- (✓) 2. Turn on the simulator and allow the temperature to reach 34°C+.2°C.
- (✓) 3. Set Intoxilyzer mode selection in the ACA mode by switching mode selection switch #9 on or selecting "C" on keyboard menu.
- (✓) 4. Attach simulator to the simulator entrance port on the Intoxilyzer.
- ✓ (✓) 5. Intoxilyzer 5000 display reads "READY TO START" or "PUSH BUTTON".
- ✓ (✓) 6. Push Start Test button or press enter on keyboard.
- ✓ (✓) 7. Insert card in response to display.
- ✓ (✓) 8. Air blank completed.
- ✓ (✓) 9. Calibration check completed. Test results 0.080 AC & 0.080 AC
- ✓ (✓) 10. Air blank completed.
- ✓ (✓) 11. When display reads Test Complete remove evidence card. Attach the card to the completed checklist.
- (✓) 12. Return mode selection switch #9 to off position after all calibration checks are complete or type Q and enter on keyboard.

SIGNATURE Jennifer A Coombs

*WITH OR WITHOUT VAPOR RECIRCULATION AND WITH OR WITHOUT KEYBOARD

DHS/DSLS/Form C116 (Rev. 7-93)

TUCSON POLICE DEPARTMENT
INTOXILYZER - ALCOHOL ANALYZER
AZ MODEL 5000 SN 66-005005
03/23/06 16:07

TEST BRAC VALUE TIME
AIR BLANK .000 16:06
INVALID SAMPLE .ND9 16:07
AIR BLANK .000 16:07

BEGIN NEW DEPRIVATION PERIOD

SUBJECT'S NAME

DULTRO
INSTRUMENT LOCATION

TIME FIRST OBSERVED

46160

OPERATOR

ADDITIONAL INFORMATION AND/OR REMARKS

Sweet Breath

INTOXILYZER INSTRUMENT PRINTER CARD

© 1986 by CMI INC.

TUCSON POLICE DEPARTMENT
INTOXILYZER - ALCOHOL ANALYZER
AZ MODEL 5000 SN 66-005005
03/23/06 16:11

TEST BRAC VALUE TIME
AIR BLANK .000 16:08
*SUBJECT TEST .187 16:11
AIR BLANK .000 16:11

* DEFICIENT SAMPLE - VALUE
PRINTED WAS HIGHEST OBTAINED.

SUBJECT'S NAME

DULTRO
INSTRUMENT LOCATION

TIME FIRST OBSERVED

46160

OPERATOR

ADDITIONAL INFORMATION AND/OR REMARKS

INTOXILYZER INSTRUMENT PRINTER CARD

© 1986 by CMI INC.

133
6 of 6
file

