



CERTIFICATION by CUSTODIAN of RECORDS  
Tucson Police Department Crime Laboratory

*TSK*

I hereby certify that these documents are a true and correct copy of the periodic maintenance\* for the Intoxilyzer 5000 Serial Number 166-005005 maintained by the Tucson Police Department Crime Laboratory pursuant to the requirements of the Arizona Department of Public Safety for a quality assurance program.

A quality assurance specialist (QAS) tested the instrument on the following dates. The acceptable accuracy limits, as defined in A.A.C. R9-14-404.A.3, for a 0.080AC solution are 0.070AC to 0.090AC.

Date: 3/23/06 Cal 1 0.080 AC Cal 2 0.080 AC

Date: 4/21/06 Cal 1 0.080 AC Cal 2 0.076 AC

Date: N/A Cal 1            AC Cal 2            AC


Between the dates of 3/23/06 and 4/21/06 the instrument was operating properly and accurately.

The instrument was taken out of service for repair on N/A.  
The instrument was returned to service on N/A.

Jennifer L. Coombs  
Jennifer L. Coombs

4/21/06

ADPS QAS Permit # QAS 29886  
SUBSCRIBED AND SWORN to before me this 21, day of April, 2006.

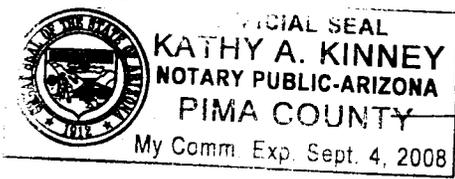

Kathy A Kinney  
Notary Public

\*Includes documents specified in A.A.C. R9-14-404.A.6

1 of 6  
JL

THIS REPORT PREPARED PURSUANT TO DUTY IMPOSED BY  
A.A.C. R9-14-404(A)

ARIZONA DEPARTMENT OF HEALTH SERVICES

STANDARD QUALITY ASSURANCE PROCEDURES *SM*  
INTOXILYZER MODEL 5000\*

AGENCY Tucson Police QA SPECIALIST Jennifer Coombs 466160  
(Print Name)

INTOXILYZER SERIAL # 66-005005 LOCATION LHB

DATE April 21 19 2006 TIME 1257

Display reads "READY TO START" or "PUSH BUTTON TO START TEST."

DIAGNOSTIC TESTS

- DVM Test check. Setting should be between .200 and .600. Mode selection switch S2 on, S1 and S3 off or keyboard menu selection "H". Reading is .538.
- Display Test check. Mode selection switch S1 on and S2 and S3 off or keyboard menu selection "V".
- Printer Test check. Mode selection switch S1, S2, S3 off or keyboard menu selection "P".
- Clock time check. Mode selection switch S10 on or keyboard menu selection "E".
- Date check. Mode selection switch S11 on or keyboard menu selection "E".

OPERATIONAL TESTS

- Alcohol free subject Test result 0.000 AC
  - Error recognition logic system functioning  
Invalid test printed
  - Proper sample recognition system  
Invalid sample printed ✓  
Deficient sample printed ✓
  - N/A Completeness of sample purge with collection tube\*\*
  - Calibration standard 0.080 AC  
Results: 0.080 AC & 0.076 AC
- Instrument operating properly and accurately. YES  NO

COMMENTS: \_\_\_\_\_  
\_\_\_\_\_

SIGNATURE Jennifer A. Coombs

0. N/A alcohol concentration standard collected for subsequent analysis.\*\*

\*WITH OR WITHOUT VAPOR RECIRCULATION AND WITH OR WITHOUT KEYBOARD  
\*\*THIS STEP IS ONLY REQUIRED IF THIS DEVICE IS BEING USED FOR SAMPLE CAPTURE.



# Tucson Police Department Crime Laboratory <sup>TS4</sup>

3 of 6  
file

TUCSON POLICE DEPARTMENT  
INTOXILYZER - ALCOHOL ANALYZER  
AZ MODEL 5000 SN 66-005005  
04/21/06 13:31

TEST	BRAC VALUE	TIME
AIR BLANK	.000	13:30
CAL. CHECK	.076	13:30
AIR BLANK	.000	13:31

SUBJECT'S NAME

LAB

INSTRUMENT LOCATION

TIME FIRST OBSERVED

46160

OPERATOR

ADDITIONAL INFORMATION AND/OR REMARKS



INTOXILYZER INSTRUMENT PRINTER CARD

© 1986 by CMI INC

TUCSON POLICE DEPARTMENT  
INTOXILYZER - ALCOHOL ANALYZER  
AZ MODEL 5000 SN 66-005005  
04/21/06 13:28

TEST	BRAC VALUE	TIME
AIR BLANK	.000	13:27
CAL. CHECK	.080	13:27
AIR BLANK	.000	13:28

SUBJECT'S NAME

LAB

INSTRUMENT LOCATION

TIME FIRST OBSERVED

46160

OPERATOR

ADDITIONAL INFORMATION AND/OR REMARKS



INTOXILYZER INSTRUMENT PRINTER CARD

© 1986 by CMI INC

4 of 6  
file

SN 66-005003  
E767.14  
INVALID TEST

04/21/86  
13:02

SAMPLE INTRODUCED  
AT IMPROPER TIME.

SUBJECT'S NAME

LAB

TIME FIRST OBSERVED

INSTRUMENT LOCATION

OPERATOR

46160

ADDITIONAL INFORMATION AND/OR REMARKS

INTOXILYZER INSTRUMENT PRINTER CARD



© 1986 by CMI INC

EXHIBIT P

5 of 6  
file

THIS REPORT PREPARED PURSUANT TO DUTY IMPOSED BY  
A.A.C. R9-14-404(A)

ARIZONA DEPARTMENT OF HEALTH SERVICES

STANDARD QUALITY ASSURANCE PROCEDURES  
INTOXILYZER MODEL 5000\*

134

STANDARD CALIBRATION CHECK PROCEDURE

Agency Tucson Police Department Date 4/21/06 Time 1257  
Intoxilyzer Serial # 66-005005 Location LAB  
QA Specialist Jennifer Coombs 4616C  
(Print Name)

- ( ✓ ) 1. Pour a standard alcohol solution of known value into a clean dry simulator jar and assemble the simulator. Insure that a tight seal has been made. Standard value: 0.080 AC
- ( ✓ ) 2. Turn on the simulator and allow the temperature to reach 34°C±.2°C.
- ( ✓ ) 3. Set Intoxilyzer mode selection in the ACA mode by switching mode selection switch #9 on or selecting "C" on keyboard menu.
- ( ✓ ) 4. Attach simulator to the simulator entrance port on the Intoxilyzer.
- ✓ ✓ 5. Intoxilyzer 5000 display reads "READY TO START" or "PUSH BUTTON".
- ✓ ✓ 6. Push Start Test button or press enter on keyboard.
- ✓ ✓ 7. Insert card in response to display.
- ✓ ✓ 8. Air blank completed.
- ✓ ✓ 9. Calibration check completed. Test results 0.080 AC & 0.076 AC
- ✓ ✓ 10. Air blank completed.
- ✓ ✓ 11. When display reads Test Complete remove evidence card. Attach the card to the completed checklist.
- ( ✓ ) 12. Return mode selection switch #9 to off position after all calibration checks are complete or type Q and enter on keyboard.

SIGNATURE Jennifer L. Coombs

\*WITH OR WITHOUT VAPOR RECIRCULATION AND WITH OR WITHOUT KEYBOARD

DHS/DSLS/Form C116 (Rev. 7-93)

TUCSON POLICE DEPARTMENT  
INTOXILYZER - ALCOHOL ANALYZER  
AZ MODEL 5000 SN 66-005005  
04/21/86 13:08

TEST BRAC VALUE TIME  
AIR BLANK .000 13:04  
\*SUBJECT TEST .100 13:07  
AIR BLANK .000 13:08

\* DEFICIENT SAMPLE - VALUE  
PRINTED WAS HIGHEST OBTAINED.

SUBJECT'S NAME \_\_\_\_\_  
LAB  
INSTRUMENT LOCATION

TIME FIRST OBSERVED \_\_\_\_\_  
46160  
OPERATOR

ADDITIONAL INFORMATION AND/OR REMARKS



INTOXILYZER INSTRUMENT PRINTER CARD

© 1986 by CMI INC.

734  
6 of 6  
file

TUCSON POLICE DEPARTMENT  
INTOXILYZER - ALCOHOL ANALYZER  
AZ MODEL 5000 SN 66-005005  
04/21/86 13:03

TEST BRAC VALUE TIME  
AIR BLANK .000 13:03  
INVALID SAMPLE .NOA 13:03  
AIR BLANK .000 13:03

BEGIN NEW DEPRIVATION PERIOD

SUBJECT'S NAME \_\_\_\_\_  
LAB  
INSTRUMENT LOCATION

TIME FIRST OBSERVED \_\_\_\_\_  
46160  
OPERATOR

ADDITIONAL INFORMATION AND/OR REMARKS

Sweet Breath



INTOXILYZER INSTRUMENT PRINTER CARD

© 1986 by CMI INC.