



CERTIFICATION by CUSTODIAN of RECORDS
Tucson Police Department Crime Laboratory

PH
8.1.08

I hereby certify that these documents are a true and correct copy of the periodic maintenance* for the Intoxilyzer 8000 Serial Number 80-000334 maintained by the Tucson Police Department Crime Laboratory pursuant to the requirements of the Arizona Department of Public Safety for a quality assurance program.

A quality assurance specialist (QAS) tested the instrument on the following dates. The acceptable accuracy limits, as defined in A.A.C. R13-10-104.A.2, for a 0.100AC solution are 0.090AC to 0.110AC.

Date: 7-31-08 Cal 1 0.100 AC Cal 2 0.098 AC

Between the dates of 7-3-08 and 7-31-08 the instrument was operating properly and accurately.

The instrument was taken out of service for repair on N/A.
The instrument was returned to service on N/A.


Clare Conley

Clare L. Conley

8-1-08

ADPS QAS Permit # 33314

SUBSCRIBED AND SWORN to before me this 1 day of August, 2008.

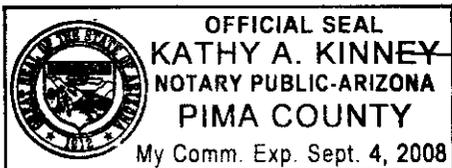

Kathy A Kinney
Notary Public

*Includes documents specified in A.A.C. R13-10-104.A.5

THIS REPORT PREPARED PURSUANT TO DUTY IMPOSED BY
A.A.C. R13-10-104(A)

ARIZONA DEPARTMENT OF PUBLIC SAFETY
STANDARD QUALITY ASSURANCE PROCEDURES
INTOXILYZER MODEL 8000
STANDARD QUALITY ASSURANCE PROCEDURE

1 of 7
cm
TSH
8.1.08

QA SPECIALIST Clare Conley AGENCY Tucson Police Department
DATE 7.31-08 TIME 0902^{cm}
INTOXILYZER SERIAL # 80-000334 LOCATION ODW-DUI SQUAD

(✓) 1. Display reads "PUSH BUTTON TO START"

DIAGNOSTIC TESTS

- (✓) 1. Clock time check.
- (✓) 2. Date check.

OPERATIONAL TESTS

- (✓) 1. Alcohol-free subject test result 0. 000 AC.
- (✓) 2. Error recognition logic system functioning.
Not a Successfully Completed Test Sequence printed
- (✓) 3. Proper sample recognition system.
Not a Successfully Completed Test Sequence printed
Deficient sample printed.
- (✓) 4. Standard Calibration Check standard 0. 100 AC
Result: 0. 0.098 AC

Instrument is operating properly and accurately. YES NO

COMMENTS None.

SIGNATURE Clare Conley

INTOXILYZER 8000
Location: TUCSON POLICE DEPT
Serial Number : 80-000334
07/31/2008

09:02:09

257
cu
154

Standard Lot#: 732503I
Last Changed By: S. CIONE #50616

QAS: S. CIONE #50616
TUCSON PD

Operator: C. CONLEY #34517
TUCSON PD

Subject: TEST, SQAP
DOB: 11/11/1111
Sex: M Weight: 111

15 Minute Deprivation Period? Yes

| Test | g/210L | Time |
|-----------------|--------|----------|
| Air Blank | 0.000 | 09:03:14 |
| Diagnostic Test | Pass | 09:03:42 |
| Air Blank | 0.000 | 09:04:09 |
| 0.100 Cal Check | 0.100 | 09:04:28 |
| Air Blank | 0.000 | 09:04:57 |
| Subject Test | 0.000 | 09:05:14 |
| Air Blank | ABT* | 09:05:20 |
| Air Blank | 0.000 | 09:05:49 |

*Sequence Aborted

Not a Successfully Completed Test Sequence

INTOXILYZER 8000
Location: TUCSON POLICE DEPT
Serial Number : 80-000334
07/31/2008

09:08:32

Standard Lot#: 732503I
Last Changed By: S. CIONE #50616

QAS: C. CONLEY #34517
TUCSON PD

Operator: C. CONLEY #34517
TUCSON PD

Subject: TEST, SQAP
DOB: 11/11/1111
Sex: M Weight: 111

15 Minute Deprivation Period? Yes

| Test | g/210L | Time |
|-----------|--------|----------|
| Air Blank | RFI* | 09:09:06 |
| Air Blank | IPS** | 09:09:21 |

*RFI Detect
**Improper Sample

Not a Successfully Completed Test Sequence

3067
du
TS4

INTOXILYZER 8000
Location: TUCSON POLICE DEPT
Serial Number : 80-000334
07/31/2008

09:09:25

4 of 7
m
BY

Standard Lot#: 732503I
Last Changed By: S. CIONE #50616

QAS: C. CONLEY #34517
TUCSON PD

Operator: C. CONLEY #34517
TUCSON PD

Subject: TEST, SQAP
DOB: 11/11/1111
Sex: M Weight: 111

15 Minute Deprivation Period? Yes

| Test | g/210L | Time |
|-----------------|--------|----------|
| Air Blank | 0.000 | 09:10:17 |
| Diagnostic Test | Pass | 09:10:44 |
| Air Blank | 0.000 | 09:11:12 |
| 0.100 Cal Check | 0.099 | 09:11:31 |
| Air Blank | 0.000 | 09:12:00 |
| Subject Test | 0.133* | 09:15:08 |
| Air Blank | 0.000 | 09:15:41 |
| Air Blank | 0.000 | 09:16:08 |
| Subject Test | XXX** | 09:16:41 |
| Air Blank | 0.000 | 09:17:15 |

*Deficient Sample

**Invalid Sample

Begin new deprivation period

Not a Successfully Completed Test Sequence

INTOXILYZER 8000
Location: TUCSON POLICE DEPT
Serial Number: 80-000334
07/31/2008

09:17:37

Standard Lot#: 732503I
Last Changed By: S. CIONE #50616

QAS: C. CONLEY #34517
TUCSON PD

| Test | g/210L | Time |
|-----------|--------|----------|
| Air Blank | 0.000 | 09:18:04 |
| Cal Check | 0.098 | 09:18:23 |
| Air Blank | 0.000 | 09:18:52 |

Clare Conley

Operator's Signature

5067
cu
154

THIS REPORT PREPARED PURSUANT TO DUTY IMPOSED BY
A.A.C. R13-10-104(A)

ARIZONA DEPARTMENT OF PUBLIC SAFETY

STANDARD QUALITY ASSURANCE PROCEDURES
INTOXILYZER MODEL 8000

STANDARD CALIBRATION CHECK PROCEDURE

b67
cu
TS4
8.1.08

QA Specialist Clare Conley AGENCY Tucson Police Department
DATE 7-31-08 TIME 0902
Intoxilyzer Serial # 80-000334 Location ODW-DUI HQ

- (✓) 1. Ensure that gas tank is attached to instrument and contains a standard alcohol concentration solution 0. 100 AC.
OR
Pour a standard alcohol concentration solution _____ AC, into a clean dry simulator and assemble the simulator. Ensure that a tight seal has been made. Turn on the simulator and allow temperature to reach 34°C ± 0.2°C
- (✓) 2. Intoxilyzer 8000 display reads "PUSH BUTTON TO START"
- (✓) 3. Go to the "Control Testing Menu". Select "D" for dry control test or "W" for wet control test. After selection is made press ENTER.
- (✓) 4. Air blank completed.
- (✓) 5. Calibration check completed. Test results 0. 100 AC.
- (✓) 6. Air blank completed.
- (✓) 7. Remove printed record. Attach the record to the completed checklist.

SIGNATURE Clare Conley

Pursuant to section 28-1327, Arizona Revised Statutes, this document is a certified duplicate of the information contained in computer storage devices of the Tucson Police Department.

INTOXILYZER 8000
Location: TUCSON POLICE DEPT
Serial Number: 80-000334
07/31/2008

09:06:16

7 of 7
en

Standard Lot#: 732503I
Last Changed By: S. CIONE #50616

154

QAS: C. CONLEY #34517
TUCSON PD

| Test | g/210L | Time |
|-----------|--------|----------|
| Air Blank | 0.000 | 09:06:43 |
| Cal Check | 0.100 | 09:07:02 |
| Air Blank | 0.000 | 09:07:32 |

Clare Conley
Operator's Signature