



CERTIFICATION by CUSTODIAN of RECORDS *TM*  
Tucson Police Department Crime Laboratory

I hereby certify that these documents are a true and correct copy of the periodic maintenance\* for the Intoxilyzer 8000 Serial Number 90-000712 maintained by the Tucson Police Department Crime Laboratory pursuant to the requirements of the Arizona Department of Public Safety for a quality assurance program.

A quality assurance specialist (QAS) tested the instrument on the following dates. The acceptable accuracy limits, as defined in A.A.C. R13-10-104.A.2, for a 0.100AC solution are 0.090AC to 0.110AC.

Date: 3.26.2007 Cal 1 0.101 AC Cal 2 0.099 AC

Between the dates of 2.26.2007 and 3.26.2007 the instrument was operating properly and accurately.

The instrument was taken out of service for repair on \_\_\_\_\_.  
The instrument was returned to service on \_\_\_\_\_.

Terry S. Gallegos

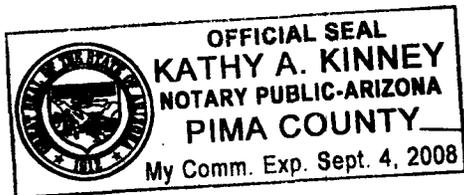
Terry S. Gallegos

April 6, 2007

ADPS QAS Permit # 33169

SUBSCRIBED AND SWORN to before me this 6<sup>th</sup>, day of

April, 2007.



Kathy A. Kinney

Notary Public

\*Includes documents specified in A.A.C. R13-10-104.A.5

EXHIBIT G-4

THIS REPORT PREPARED PURSUANT TO DUTY IMPOSED BY  
A.A.C. R13-10-104(A)

10 of 7  
TSB  
4/17

ARIZONA DEPARTMENT OF PUBLIC SAFETY

STANDARD QUALITY ASSURANCE PROCEDURES  
INTOXILYZER MODEL 8000

STANDARD QUALITY ASSURANCE PROCEDURE

QA SPECIALIST Terry Gallegos 28847 AGENCY Tucson Police Department  
DATE 3.26.2007 TIME 1646  
INTOXILYZER SERIAL # 80-000712 LOCATION DUI HQ

( ✓ ) 1. Display reads "PUSH BUTTON TO START"

DIAGNOSTIC TESTS

- ( ✓ ) 1. Clock time check.
- ( ✓ ) 2. Date check.

OPERATIONAL TESTS

- ( ✓ ) 1. Alcohol-free subject test result 0. 000 AC.
- ( ✓ ) 2. Error recognition logic system functioning.  
Not a Successfully Completed Test Sequence printed ✓✓✓
- ( ✓ ) 3. Proper sample recognition system.  
Not a Successfully Completed Test Sequence printed  
Deficient sample printed.
- ( ✓ ) 4. Standard Calibration Check standard 0. 100 AC  
Result: 0. 099 AC

Instrument is operating properly and accurately. YES  NO

COMMENTS

---



---



---



---

SIGNATURE Terry Gallegos

Pursuant to section 28-1327, Arizona Revised Statutes, this document is a certified duplicate of the information contained in computer storage devices of the Tucson Police Department.

INTOXILYZER 8000  
Location: TUCSON POLICE DEPT  
Serial Number : 80-000712  
03/26/2007

16:48:11

2087  
TSY mm

---

Standard Lot#: 635301I  
Last Changed By: G. EPPLEY #26227

---

QAS: T. GALLEGOS #28847  
TUCSON PD CRIME LAB

---

Operator: T. GALLEGOS #28847  
TUCSON PD CRIME LAB

---

Subject: SQAP, SQAP  
DOB: 11/11/1111  
Sex: F Weight: 111

---

15 Minute Deprivation Period? Yes

---

Test	g/210L	Time
Air Blank	0.000	16:48:59
Diagnostic Test	Pass	16:49:27
Air Blank	0.000	16:49:54
0.100 Cal Check	0.100	16:50:13
Air Blank	0.000	16:50:42
Subject Test	0.000	16:51:02
Air Blank	0.000	16:51:30
Five Minute Wait	ABT*	
Air Blank	0.000	16:52:04

\*Sequence Aborted

**Not a Successfully Completed Test Sequence**

INTOXILYZER 8000  
Location: TUCSON POLICE DEPT  
Serial Number : 80-000712  
03/26/2007

16:52:10

3 of 7  
TSG/m

---

Standard Lot#: 635301I  
Last Changed By: G. EPPLEY #26227

---

QAS: T. GALLEGOS #28847  
TUCSON PD CRIME LAB

---

Operator: T. GALLEGOS #28847  
TUCSON PD CRIME LAB

---

Subject: SQAP, SQAP  
DOB: 11/11/1111  
Sex: F Weight: 111

---

15 Minute Deprivation Period? Yes

---

Test	g/210L	Time
Air Blank	0.000	16:52:58
Diagnostic Test	Pass	16:53:26
Air Blank	0.000	16:53:53
0.100 Cal Check	0.100	16:54:12
Air Blank	RFI*	16:54:20
Air Blank	IPS**	16:54:28

\*RFI Detect

\*\*Improper Sample

**Not a Successfully Completed Test Sequence**

INTOXILYZER 8000  
Location: TUCSON POLICE DEPT  
Serial Number : 80-000712  
03/26/2007

16:54:53

4 of 7  
TSJ mm

Standard Lot#: 635301I  
Last Changed By: G. EPPLEY #26227

QAS: T. GALLEGOS #28847  
TUCSON PD CRIME LAB

Operator: T. GALLEGOS #28847  
TUCSON PD CRIME LAB

Subject: SQAP, SQAP  
DOB: 11/11/1111  
Sex: F Weight: 111

15 Minute Deprivation Period? Yes

Test	g/210L	Time
Air Blank	0.000	16:55:42
Diagnostic Test	Pass	16:56:09
Air Blank	0.000	16:56:36
0.100 Cal Check	0.101	16:56:55
Air Blank	0.000	16:57:25
Subject Test	0.116*	17:00:33
Air Blank	0.000	17:01:05
Air Blank	0.000	17:01:32
Subject Test	XXX**	17:02:00
Air Blank	0.000	17:02:33

\*Deficient Sample

\*\*Invalid Sample

Begin new deprivation period

**Not a Successfully Completed Test Sequence**

INTOXILYZER 8000

Location: TUCSON POLICE DEPT

Serial Number: 80-000712

03/26/2007

17:03:01

Sof 7  
TS4 mm

-----  
Standard Lot#: 635301I

Last Changed By: G. EPPLEY #26227

-----  
QAS: T. GALLEGOS #28847

TUCSON PD CRIME LAB  
-----

Test	g/210L	Time
Air Blank	0.000	17:03:28
Cal Check	0.099	17:03:47
Air Blank	0.000	17:04:17

  
-----  
Operator's Signature

EXHIBIT G-2

THIS REPORT PREPARED PURSUANT TO DUTY IMPOSED BY  
A.A.C. R13-10-104(A)

ARIZONA DEPARTMENT OF PUBLIC SAFETY  
STANDARD QUALITY ASSURANCE PROCEDURES  
INTOXILYZER MODEL 8000

60 of 7  
Dy 7/17

STANDARD CALIBRATION CHECK PROCEDURE

QA Specialist Terry Gallegos 28847 AGENCY Tucson Police Department  
DATE 3-26-2007 TIME 1646  
Intoxilyzer Serial # 80-000712 Location DUI HQ

- (✓) 1. Ensure that gas tank is attached to instrument and contains a standard alcohol concentration solution 0. 100 AC.  
OR  
Pour a standard alcohol concentration solution \_\_\_\_\_ AC, into a clean dry simulator and assemble the simulator. Ensure that a tight seal has been made. Turn on the simulator and allow temperature to reach 34°C ± 0.2°C
- (✓) 2. Intoxilyzer 8000 display reads "PUSH BUTTON TO START"
- (✓) 3. Go to the "Control Testing Menu". Select "D" for dry control test or "W" for wet control test. After selection is made press ENTER.
- (✓) 4. Air blank completed.
- (✓) 5. Calibration check completed. Test results 0. 101 AC.
- (✓) 6. Air blank completed.
- (✓) 7. Remove printed record. Attach the record to the completed checklist.

SIGNATURE Terry Gallegos

DPS Form Exh G-2 (Rev. 05-01)

INTOXILYZER 8000

Location: TUCSON POLICE DEPT

Serial Number: 80-000712

03/26/2007

16:46:48

7097

TJH

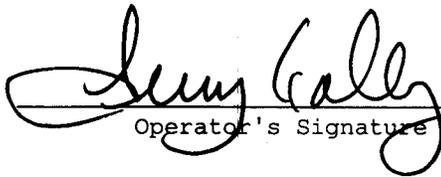
-----  
Standard Lot#: 635301I

Last Changed By: G. EPPLEY #26227  
-----

QAS: T. GALLEGOS #28847

TUCSON PD CRIME LAB  
-----

Test	g/210L	Time
Air Blank	0.000	16:47:16
Cal Check	0.101	16:47:34
Air Blank	0.000	16:48:04

  
Operator's Signature



TUCSON POLICE DEPARTMENT  
CRIME LABORATORY

INTOXILYZER SERVICE RECORD  
FOR  
CALIBRATION GAS TANK CHANGE

10/2  
mm

Date: 031507

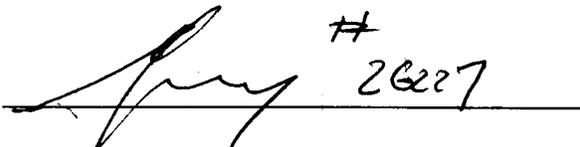
QAS: Eppley 2627

Intoxilyzer Serial Number: 80-000712

New Lot Number: 635301 I

New Expiration Date: 122108

- (X) 1. Intoxilyzer 8000 display reads "PUSH BUTTON TO START"
- (X) 2. Remove the old gas tank and install the new one.
- (X) 3. Hit the "ESC" key twice and swipe the QAS card.
- (X) 4. Go to the "M-Maintenance" menu and select "S-Standard Change."  
Select "D" for dry gas and enter the following information:  
 Enter Target Value: 0.100  
 Enter Control Lot #: From the tank label  
 Enter Exp Date: From the tank label (mm/dd/yyyy)  
 Edit info Y/N? Y or N  
 Update Std Info? Y ENTER  
 "Please wait saving..."
- (X) 5. Hit the "ESC" key twice.
- (X) 6. Go to the "M-Maintenance" menu and select "T-Control Testing."  
Select "D" for dry control test. After selection is made press ENTER.
- (X) 7. Air blank completed.
- (X) 8. Calibration check completed. Test results 0. 101 AC.
- (X) 9. Air blank completed.
- (X) 10. Remove and sign printed record. Attach the record to the completed checklist.

SIGNATURE  # 2627

2 of 2

Bh mm

INTOXILYZER 8000  
Location: TUCSON POLICE DEPT  
Serial Number: 88-000712  
03/15/2007 21:41:39

Standard Lot#: 6353011  
Last Changed By: G. EPPLEY #26227

OAS: G. EPPLEY #26227  
TUCSON PD

Test	g/210L	Time
Air Blank	0.000	21:41:37
Cal Check	0.101	21:41:55
Air Blank	0.000	21:42:25

  
Operator's Signature