



CERTIFICATION by CUSTODIAN of RECORDS

Tucson Police Department Crime Laboratory  
270 S. Stone Avenue Tucson, AZ 85701-1917

Tby  
12-17-09

I hereby certify that these documents are a true and correct copy of the periodic maintenance\* for the Intoxilyzer 8000 Serial Number 80-001108 maintained by the Tucson Police Department Crime Laboratory pursuant to the requirements of the Arizona Department of Public Safety for a quality assurance program.

A quality assurance specialist (QAS) tested the instrument on the following dates. The acceptable accuracy limits, as defined in A.A.C. R13-10-104.A.2, for a 0.100AC solution are 0.090AC to 0.110AC.

Date: 12/17/09 Cal 1 0.102 AC Cal 2 0.100 AC

Between the dates of 11/19/09 and 12/17/09 the instrument was operating properly and accurately.

The instrument was taken out of service for repair on N/A.  
The instrument was returned to service on N/A.

Cheryl K. Straub

Cheryl K. Straub


12/17/09

ADPS QAS Permit # 33408

SUBSCRIBED AND SWORN to before me this 17<sup>th</sup>, day of December, 2009.

A.M. Hernandez

Notary Public

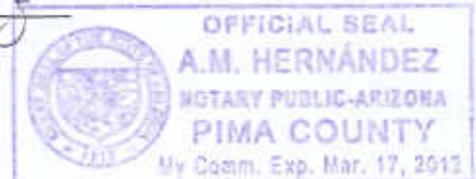

\*Includes documents specified in A.A.C. R13-10-104.A.5

THIS REPORT PREPARED PURSUANT TO DUTY IMPOSED BY  
A.A.C. R13-10-104(A)

ARIZONA DEPARTMENT OF PUBLIC SAFETY

STANDARD QUALITY ASSURANCE PROCEDURES  
INTOXILYZER MODEL 8000

STANDARD QUALITY ASSURANCE PROCEDURE

TS4  
12-17-09

QA SPECIALIST Cheryl Straub AGENCY Tucson Police Department

DATE 12/17/09 TIME 06:20

INTOXILYZER SERIAL # 80-001108 LOCATION TEAM IV

(  ) 1. Display reads "PUSH BUTTON TO START"

DIAGNOSTIC TESTS

- (  ) 1. Clock time check.
- (  ) 2. Date check.

OPERATIONAL TESTS

- (  ) 1. Alcohol-free subject test result 0. 000 AC.
- (  ) 2. Error recognition logic system functioning.  
Not a Successfully Completed Test Sequence printed
- (  ) 3. Proper sample recognition system.  
Not a Successfully Completed Test Sequence printed  
Deficient sample printed.
- (  ) 4. Standard Calibration Check standard 0. 100 AC  
Result: 0. 100 AC

Instrument is operating properly and accurately. YES  NO

COMMENTS

\_\_\_\_\_  
\_\_\_\_\_  
\_\_\_\_\_  
\_\_\_\_\_

SIGNATURE Cheryl Straub

277  
CS

INTOXILYZER 8000  
Location: ARIZONA  
Serial Number : 80-001108  
12/17/2009

06:24:56

TD4

Standard Lot#: 642845  
Last Changed By: C. STRAUB #50772

QAS: C. STRAUB #50772  
TUCSON PD

Operator: C. STRAUB #50772  
TUCSON PD

Subject: SQAP, SQAP  
DOB: 11/11/1111  
Sex: F Weight: 111

15 Minute Deprivation Period? Yes

Test	g/210L	Time
Air Blank	0.000	06:26:00
Diagnostic Test	Pass	06:26:27
Air Blank	0.000	06:26:55
0.100 Cal Check	0.102	06:27:13
Air Blank	0.000	06:27:43
Subject Test	0.000	06:28:12
Air Blank	ABT*	06:28:20
Air Blank	0.000	06:28:48

\*Sequence Aborted

**Not a Successfully Completed Test Sequence**

377  
CS

INTOXILYZER 8000  
Location: ARIZONA  
Serial Number : 80-001108  
12/17/2009

06:29:18

154

Standard Lot#: 642845  
Last Changed By: C. STRAUB #50772

QAS: C. STRAUB #50772  
TUCSON PD

Operator: C. STRAUB #50772  
TUCSON PD

Subject: SQAP, SQAP  
DOB: 11/11/1111  
Sex: F Weight: 111

15 Minute Deprivation Period? Yes

Test	g/210L	Time
Air Blank	RFI*	06:29:54
Air Blank	IPS**	06:30:06

\*RFI Detect  
\*\*Improper Sample

**Not a Successfully Completed Test Sequence**

477  
CS

INTOXILYZER 8000  
Location: ARIZONA  
Serial Number : 80-001108  
12/17/2009

06:30:40

BY

Standard Lot#: 642845  
Last Changed By: C. STRAUB #50772

QAS: C. STRAUB #50772  
TUCSON PD

Operator: C. STRAUB #50772  
TUCSON PD

Subject: SQAP, SQAP  
DOB: 11/11/1111  
Sex: F Weight: 111

15 Minute Deprivation Period? Yes

Test	g/210L	Time
Air Blank	0.000	06:31:38
Diagnostic Test	Pass	06:32:05
Air Blank	0.000	06:32:32
0.100 Cal Check	0.103	06:32:51
Air Blank	0.000	06:33:20
Subject Test	0.116*	06:36:29
Air Blank	0.000	06:37:02
Air Blank	0.000	06:37:30
Subject Test	XXX**	06:38:17
Air Blank	0.000	06:38:50

\*Deficient Sample

\*\*Invalid Sample

Begin new deprivation period

**Not a Successfully Completed Test Sequence**

577  
CS

INTOXILYZER 8000  
Location: ARIZONA  
Serial Number: 80-001108  
12/17/2009 06:42:44

154

-----  
Standard Lot#: 642845  
Last Changed By: C. STRAUB #50772  
-----

QAS: C. STRAUB #50772  
TUCSON PD  
-----

Test	g/210L	Time
Air Blank	0.000	06:43:11
Cal Check	0.100	06:43:30
Air Blank	0.000	06:43:59



Operator's Signature

EXHIBIT G-2

697  
CS

THIS REPORT PREPARED PURSUANT TO DUTY IMPOSED BY  
A.A.C. R13-10-104(A)

ARIZONA DEPARTMENT OF PUBLIC SAFETY

STANDARD QUALITY ASSURANCE PROCEDURES  
INTOXILYZER MODEL 8000

TSY  
12-17-09

STANDARD CALIBRATION CHECK PROCEDURE

QA Specialist Cheryl STRAUB AGENCY Tucson Police Department  
DATE 12/17/09 TIME 06:20  
Intoxilyzer Serial # 80-001108 Location TEAM IV

- ( ✓ ) 1. Ensure that gas tank is attached to instrument and contains a standard alcohol concentration solution 0. 100 AC.  
OR  
Pour a standard alcohol concentration solution N/A AC, into a clean dry simulator and assemble the simulator. Ensure that a tight seal has been made. Turn on the simulator and allow temperature to reach 34°C ± 0.2°C
- ( ✓ ) 2. Intoxilyzer 8000 display reads "PUSH BUTTON TO START"
- ( ✓ ) 3. Go to the "Control Testing Menu". Select "D" for dry control test or "W" for wet control test. After selection is made press ENTER.
- ( ✓ ) 4. Air blank completed.
- ( ✓ ) 5. Calibration check completed. Test results 0. 102 AC.
- ( ✓ ) 6. Air blank completed.
- ( ✓ ) 7. Remove printed record. Attach the record to the completed checklist.

SIGNATURE Cheryl Straub

DPS Form Exh G-2 (Rev. 05-01)

797  
CS


INTOXILYZER 8000  
Location: ARIZONA  
Serial Number: 80-001108  
12/17/2009 06:20:13

154

-----  
Standard Lot#: 642845  
Last Changed By: C. STRAUB #50772  
-----

QAS: C. STRAUB #50772  
TUCSON PD  
-----

Test	g/210L	Time
Air Blank	0.000	06:20:40
Cal Check	0.102	06:20:59
Air Blank	0.000	06:21:29

  
-----  
Operator's Signature