



CERTIFICATION by CUSTODIAN of RECORDS

Tucson Police Department Crime Laboratory
270 S. Stone Avenue Tucson, AZ 85701-1917

SC
6/7/10

I hereby certify that these documents are a true and correct copy of the periodic maintenance* for the Intoxilyzer 8000 Serial Number 80-001163 maintained by the Tucson Police Department Crime Laboratory pursuant to the requirements of the Arizona Department of Public Safety for a quality assurance program.

A quality assurance specialist (QAS) tested the instrument on the following dates. The acceptable accuracy limits, as defined in A.A.C. R13-10-104.A.2, for a 0.100AC solution are 0.090AC to 0.110AC.

Date: 6.3.2010 Cal 1 0.100 AC Cal 2 0.099 AC

Between the dates of 5.6.2010 and 6.3.2010 the instrument was operating properly and accurately.

The instrument was taken out of service for repair on .
The instrument was returned to service on .

Terry Gallegos

Terry S. Gallegos


6.7.2010

ADPS QAS Permit # 33169

SUBSCRIBED AND SWORN to before me this 7, day of June, 2010.

A.M. Hernandez

Notary Public

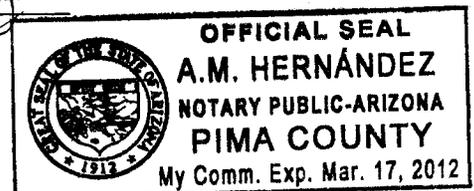

*Includes documents specified in A.A.C. R13-10-104.A.5

EXHIBIT G-4

THIS REPORT PREPARED PURSUANT TO DUTY IMPOSED BY
A.A.C. R13-10-104(A)

ARIZONA DEPARTMENT OF PUBLIC SAFETY

STANDARD QUALITY ASSURANCE PROCEDURES
INTOXILYZER MODEL 8000

STANDARD QUALITY ASSURANCE PROCEDURE

10f7
TS4
SC
6/7/10

QA SPECIALIST Terry Gallegos 28847 AGENCY Tucson Police Department

DATE 6-3-2010 TIME 1525

INTOXILYZER SERIAL # 80-001163 LOCATION Crime Lab

() 1. Display reads "PUSH BUTTON TO START"

DIAGNOSTIC TESTS

- () 1. Clock time check.
- () 2. Date check.

OPERATIONAL TESTS

- () 1. Alcohol-free subject test result 0. 000 AC.
- () 2. Error recognition logic system functioning.
Not a Successfully Completed Test Sequence printed ✓✓
- () 3. Proper sample recognition system.
Not a Successfully Completed Test Sequence printed ✓
Deficient sample printed.
- () 4. Standard Calibration Check standard 0. 100 AC
Result: 0. 099 AC

Instrument is operating properly and accurately. YES NO

COMMENTS

SIGNATURE Terry Gallegos

Pursuant to section 28-1327, Arizona Revised Statutes, this document is a certified duplicate of the information contained in computer storage devices of the Tucson Police Department.

INTOXILYZER 8000
Location: ARIZONA
Serial Number : 80-001163
06/03/2010

15:26:42

2 of 7
154
5C

Standard Lot#: 642845
Last Changed By: C. STRAUB #50772

QAS: T. GALLEGOS #28847
TUCSON PD CRIME LAB

Operator: T. GALLEGOS #28847
TUCSON PD CRIME LAB

Subject: TEST, SQAP
DOB: 11/11/1111
Sex: F Weight: 111

15 Minute Deprivation Period? Yes

Test	g/210L	Time
Air Blank	0.000	15:27:38
Diagnostic Test	Pass	15:28:05
Air Blank	0.000	15:28:32
0.100 Cal Check	0.100	15:28:51
Air Blank	0.000	15:29:21
Subject Test	0.000	15:29:40
Air Blank	ABT*	15:29:49
Air Blank	0.000	15:30:18

*Sequence Aborted

Not a Successfully Completed Test Sequence

INTOXILYZER 8000
Location: ARIZONA
Serial Number : 80-001163
06/03/2010 15:30:33

3087
TS4

SC

Standard Lot#: 642845
Last Changed By: C. STRAUB #50772

QAS: T. GALLEGOS #28847
TUCSON PD CRIME LAB

Operator: T. GALLEGOS #28847
TUCSON PD CRIME LAB

Subject: SQAP,TEST
DOB: 11/11/1111
Sex: F Weight: 111

15 Minute Deprivation Period? Yes

Test	g/210L	Time
Air Blank	0.000	15:31:45
Diagnostic Test	Pass	15:32:12
Air Blank	0.000	15:32:39
0.100 Cal Check	0.100	15:32:58
Air Blank	RFI*	15:33:08
Air Blank	IPS**	15:33:16

*RFI Detect
**Improper Sample

Not a Successfully Completed Test Sequence

INTOXILYZER 8000
Location: ARIZONA
Serial Number : 80-001163
06/03/2010 15:34:36

4087
B4
SC

Standard Lot#: 642845
Last Changed By: C. STRAUB #50772

QAS: T. GALLEGOS #28847
TUCSON PD CRIME LAB

Operator: T. GALLEGOS #28847
TUCSON PD CRIME LAB

Subject: TEST, SQAP
DOB: 11/11/1111
Sex: F Weight: 111

15 Minute Deprivation Period? Yes

Test	g/210L	Time
Air Blank	0.000	15:35:28
Diagnostic Test	Pass	15:35:55
Air Blank	0.000	15:36:22
0.100 Cal Check	0.099	15:36:41
Air Blank	0.000	15:37:11
Subject Test	0.311*	15:40:19
Air Blank	0.000	15:40:53
Air Blank	0.000	15:41:20
Subject Test	XXX**	15:41:43
Air Blank	0.000	15:42:17

*Deficient Sample
**Invalid Sample
Begin new deprivation period

Not a Successfully Completed Test Sequence

Pursuant to section 28-1327, Arizona Revised Statutes, this document is a certified duplicate of the information contained in computer storage devices of the Tucson Police Department.


INTOXILYZER 8000
Location: ARIZONA
Serial Number: 80-001163
06/03/2010 15:42:38

Standard Lot#: 642845
Last Changed By: C. STRAUB #50772

QAS: T. GALLEGOS #28847
TUCSON PD CRIME LAB

5087
734
SC

Test	g/210L	Time
Air Blank	0.000	15:43:05
Cal Check	0.099	15:43:24
Air Blank	0.000	15:43:54



Operator's Signature

EXHIBIT G-2

THIS REPORT PREPARED PURSUANT TO DUTY IMPOSED BY
A.A.C. R13-10-104(A)

ARIZONA DEPARTMENT OF PUBLIC SAFETY

STANDARD QUALITY ASSURANCE PROCEDURES
INTOXILYZER MODEL 8000

STANDARD CALIBRATION CHECK PROCEDURE

6077
124 SC
6/7/10

QA Specialist Terry Gallegos 28847 AGENCY Tucson Police Department
DATE 6-3-2010 TIME 1525
Intoxilyzer Serial # 80-001163 Location CrimeLab

- (✓) 1. Ensure that gas tank is attached to instrument and contains a standard alcohol concentration solution 0. 100 AC.
OR
Pour a standard alcohol concentration solution _____ AC, into a clean dry simulator and assemble the simulator. Ensure that a tight seal has been made. Turn on the simulator and allow temperature to reach 34°C ± 0.2°C
- (✓) 2. Intoxilyzer 8000 display reads "PUSH BUTTON TO START"
- (✓) 3. Go to the "Control Testing Menu". Select "D" for dry control test or "W" for wet control test. After selection is made press ENTER.
- (✓) 4. Air blank completed.
- (✓) 5. Calibration check completed. Test results 0. 100 AC.
- (✓) 6. Air blank completed.
- (✓) 7. Remove printed record. Attach the record to the completed checklist.

SIGNATURE Terry Gallegos

DPS Form Exh G-2 (Rev. 05-01)

Pursuant to section 28-1327, Arizona Revised Statutes, this document is a certified duplicate of the information contained in computer storage devices of the Tucson Police Department.


INTOXILYZER 8000
Location: ARIZONA
Serial Number: 80-001163
06/03/2010 15:25:17

Standard Lot#: 642845
Last Changed By: C. STRAUB #50772

QAS: T. GALLEGOS #28847
TUCSON PD CRIME LAB

Test	g/210L	Time
Air Blank	0.000	15:25:45
Cal Check	0.100	15:26:03
Air Blank	0.000	15:26:33

7067
784
SC



Operator's Signature