



CERTIFICATION by CUSTODIAN of RECORDS

Tucson Police Department Crime Laboratory
270 S. Stone Avenue Tucson, AZ 85701-1917

TS4
9-2-2010

I hereby certify that these documents are a true and correct copy of the periodic maintenance* for the Intoxilyzer 8000 Serial Number 80-001163 maintained by the Tucson Police Department Crime Laboratory pursuant to the requirements of the Arizona Department of Public Safety for a quality assurance program.

A quality assurance specialist (QAS) tested the instrument on the following dates. The acceptable accuracy limits, as defined in A.A.C. R13-10-104.A.2, for a 0.100AC solution are 0.090AC to 0.110AC.

Date: 08/26/10 Cal 1 0.097 AC Cal 2 0.098 AC

Between the dates of 07/29/10 and 08/26/10 the instrument was operating properly and accurately.

The instrument was taken out of service for repair on N/A.
The instrument was returned to service on N/A.

Cheryl K. Straub

Cheryl K. Straub


08/31/10

ADPS QAS Permit # 33408

SUBSCRIBED AND SWORN to before me this 31, day of August, 2010.

A.M. Hernández

Notary Public

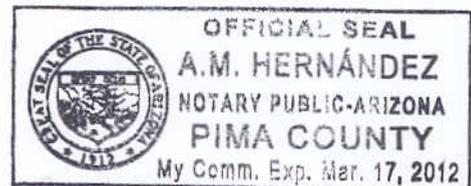

*Includes documents specified in A.A.C. R13-10-104.A.5

197
CS

THIS REPORT PREPARED PURSUANT TO DUTY IMPOSED BY
A.A.C. R13-10-104(A)

ARIZONA DEPARTMENT OF PUBLIC SAFETY

STANDARD QUALITY ASSURANCE PROCEDURES
INTOXILYZER MODEL 8000

TSK

STANDARD QUALITY ASSURANCE PROCEDURE

9-2-2010

QA SPECIALIST Cheryl Straub AGENCY Tucson Police Department
DATE 08/26/10 TIME 11:27
INTOXILYZER SERIAL # 80-001163 LOCATION CRIME LAB

(✓) 1. Display reads "PUSH BUTTON TO START"

DIAGNOSTIC TESTS

- (✓) 1. Clock time check.
- (✓) 2. Date check.

OPERATIONAL TESTS

- (✓) 1. Alcohol-free subject test result 0. 000 AC.
- (✓) 2. Error recognition logic system functioning.
Not a Successfully Completed Test Sequence printed
- (✓) 3. Proper sample recognition system.
Not a Successfully Completed Test Sequence printed
Deficient sample printed.
- (✓) 4. Standard Calibration Check standard 0. 100 AC
Result: 0. 098 AC

Instrument is operating properly and accurately. YES NO

COMMENTS

SIGNATURE

Cheryl Straub

297
CS

134

INTOXILYZER 8000
Location: ARIZONA
Serial Number : 80-001163
08/26/2010

11:28:36

Standard Lot#: 719919
Last Changed By: S. CIONE #50616

QAS: C. STRAUB #50772
TUCSON PD

Operator: C. STRAUB #50772
TUCSON PD

Subject: SQAP, SQAP
DOB: 11/11/1111
Sex: F Weight: 111

15 Minute Deprivation Period? Yes

Test	g/210L	Time
Air Blank	0.000	11:29:26
Diagnostic Test	Pass	11:29:53
Air Blank	0.000	11:30:21
0.100 Cal Check	0.097	11:30:39
Air Blank	0.000	11:31:09
Subject Test	0.000	11:31:29
Air Blank	ABT*	11:31:37
Air Blank	0.000	11:32:05

*Sequence Aborted

Not a Successfully Completed Test Sequence

377
CS

B4

INTOXILYZER 8000
Location: ARIZONA
Serial Number : 80-001163
08/26/2010

11:32:12

Standard Lot#: 719919
Last Changed By: S. CIONE #50616

QAS: C. STRAUB #50772
TUCSON PD

Operator: C. STRAUB #50772
TUCSON PD

Subject: SQAP, SQAP
DOB: 11/11/1111
Sex: F Weight: 111

15 Minute Deprivation Period? Yes

Test	g/210L	Time
Air Blank	RFI*	11:32:48
Air Blank	IPS**	11:32:55

*RFI Detect
**Improper Sample

Not a Successfully Completed Test Sequence

477
CS
B4

INTOXILYZER 8000
Location: ARIZONA
Serial Number : 80-001163
08/26/2010 11:33:00

Standard Lot#: 719919
Last Changed By: S. CIONE #50616

QAS: C. STRAUB #50772
TUCSON PD

Operator: C. STRAUB #50772
TUCSON PD

Subject: SQAP, SQAP
DOB: 11/11/1111
Sex: F Weight: 111

15 Minute Deprivation Period? Yes

Test	g/210L	Time
Air Blank	0.000	11:33:50
Diagnostic Test	Pass	11:34:18
Air Blank	0.000	11:34:45
0.100 Cal Check	0.099	11:35:04
Air Blank	0.000	11:35:34
Subject Test	0.146*	11:38:42
Air Blank	0.000	11:39:14
Air Blank	0.000	11:39:42
Subject Test	XXX**	11:40:30
Air Blank	0.000	11:41:04

*Deficient Sample

**Invalid Sample

Begin new deprivation period

Not a Successfully Completed Test Sequence

587
CS


TS4

INTOXILYZER 8000
Location: ARIZONA
Serial Number: 80-001163
08/26/2010 11:41:30

Standard Lot#: 719919
Last Changed By: S. CIONE #50616

QAS: C. STRAUB #50772
TUCSON PD

Test	g/210L	Time
Air Blank	0.000	11:41:57
Cal Check	0.098	11:42:16
Air Blank	0.000	11:42:47



Operator's Signature

THIS REPORT PREPARED PURSUANT TO DUTY IMPOSED BY
A.A.C. R13-10-104(A)

ARIZONA DEPARTMENT OF PUBLIC SAFETY

154

STANDARD QUALITY ASSURANCE PROCEDURES
INTOXILYZER MODEL 8000

9-2-2010

STANDARD CALIBRATION CHECK PROCEDURE

QA Specialist Cheryl STRAUB AGENCY Tucson Police Department
DATE 08/26/10 TIME 11:27
Intoxilyzer Serial # 80-001163 Location CRIME LAB

- (✓) 1. Ensure that gas tank is attached to instrument and contains a standard alcohol concentration solution 0. 100 AC.
OR
Pour a standard alcohol concentration solution N/A AC, into a clean dry simulator and assemble the simulator. Ensure that a tight seal has been made. Turn on the simulator and allow temperature to reach $34^{\circ}\text{C} \pm 0.2^{\circ}\text{C}$
- (✓) 2. Intoxilyzer 8000 display reads "PUSH BUTTON TO START"
- (✓) 3. Go to the "Control Testing Menu". Select "D" for dry control test or "W" for wet control test. After selection is made press ENTER.
- (✓) 4. Air blank completed.
- (✓) 5. Calibration check completed. Test results 0. 097 AC.
- (✓) 6. Air blank completed.
- (✓) 7. Remove printed record. Attach the record to the completed checklist.

SIGNATURE

Cheryl Straub

DPS Form Exh G-2 (Rev. 05-01)

777
CS


154

INTOXILYZER 8000
Location: ARIZONA
Serial Number: 80-001163
08/26/2010 11:27:10

Standard Lot#: 719919
Last Changed By: S. CIONE #50616

QAS: C. STRAUB #50772
TUCSON PD

Test	g/210L	Time
Air Blank	0.000	11:27:37
Cal Check	0.097	11:27:56
Air Blank	0.000	11:28:26



Operator's Signature