



CERTIFICATION by CUSTODIAN of RECORDS

Tucson Police Department Crime Laboratory
270 S. Stone Avenue Tucson, AZ 85701-1917

By
4-13-09

I hereby certify that these documents are a true and correct copy of the periodic maintenance* for the Intoxilyzer 8000 Serial Number 80-001108 maintained by the Tucson Police Department Crime Laboratory pursuant to the requirements of the Arizona Department of Public Safety for a quality assurance program.

A quality assurance specialist (QAS) tested the instrument on the following dates. The acceptable accuracy limits, as defined in A.A.C. R13-10-104.A.2, for a 0.100AC solution are 0.090AC to 0.110AC.

Date: — Cal 1 N/A AC Cal 2 N/A AC

Between the dates of N/A and N/A the instrument was operating properly and accurately.

The instrument was taken out of service for repair on 3/7/09.
The instrument was returned to service on —.

Sarah Cione

Sarah L. Cione


4/13/09

ADPS QAS Permit # 33355

SUBSCRIBED AND SWORN to before me this 13, day of April, 2009.

A. Hernandez

Notary Public

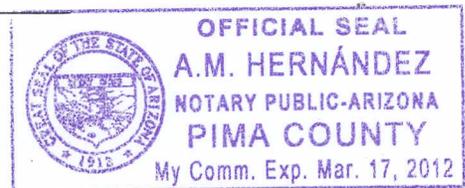

*Includes documents specified in A.A.C. R13-10-104.A.5



TUCSON POLICE DEPARTMENT
CRIME LABORATORY

1 of 15c

INTOXILYZER SERVICE RECORD

TS4
4-13-09

Date: 3/7/09

QAS: Sarah Cione

Intoxilyzer Serial Number: 80-001108

Reason For Service: regulator not recognized as having pressure
even though gas tank was not empty. Instrument worked fine
with another regulator, but no spare regulator available

Date Out of Service: 3/7/09

Calibration Check completed prior to removal from service

Date: 3/6/09

SQAP completed prior to removal from service

Date: 3/6/09

Corrective Action: Sent to CMI, Inc.

sent in regulator (not instrument) to be repaired