



CERTIFICATION by CUSTODIAN of RECORDS
Tucson Police Department Crime Laboratory

154
8-29-08

I hereby certify that these documents are a true and correct copy of the periodic maintenance* for the Intoxilyzer 8000 Serial Number 80-002201 maintained by the Tucson Police Department Crime Laboratory pursuant to the requirements of the Arizona Department of Public Safety for a quality assurance program.

A quality assurance specialist (QAS) tested the instrument on the following dates. The acceptable accuracy limits, as defined in A.A.C. R13-10-104.A.2, for a 0.100AC solution are 0.090AC to 0.110AC.

Date: 8-28-08 Cal 1 0.097 AC Cal 2 0.096 AC

Between the dates of 7-31-08 and 8-28-08 the instrument was operating properly and accurately.

The instrument was taken out of service for repair on N/A
The instrument was returned to service on N/A


Clare Conley

Clare L. Conley

8-29-08

ADPS QAS Permit # 33314

SUBSCRIBED AND SWORN to before me this 29th day of August, 2008.

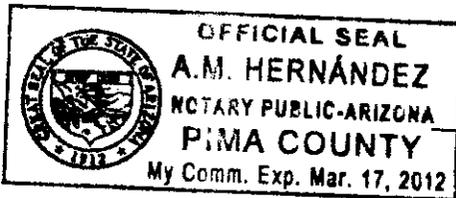

Ant Hernandez

Notary Public

*Includes documents specified in A.A.C. R13-10-104.A.5

Pursuant to section 28-1327, Arizona Revised Statutes, this document is a certified duplicate of the information contained in computer storage devices of the Tucson Police Department.

THIS REPORT PREPARED PURSUANT TO DUTY IMPOSED BY
A.A.C. R13-10-104(A)

ARIZONA DEPARTMENT OF PUBLIC SAFETY

STANDARD QUALITY ASSURANCE PROCEDURES
INTOXILYZER MODEL 8000

STANDARD QUALITY ASSURANCE PROCEDURE

1 of 7
cu
py 8.29.08

QA SPECIALIST Clare Conley AGENCY Tucson Police Department

DATE 8-28-08 TIME 1213

INTOXILYZER SERIAL # 80-002201 LOCATION Vehicle #817

(✓) 1. Display reads "PUSH BUTTON TO START"

DIAGNOSTIC TESTS

(✓) 1. Clock time check.

(✓) 2. Date check.

OPERATIONAL TESTS

(✓) 1. Alcohol-free subject test result 0. 000 AC.

(✓) 2. Error recognition logic system functioning.
Not a Successfully Completed Test Sequence printed

(✓) 3. Proper sample recognition system.
Not a Successfully Completed Test Sequence printed
Deficient sample printed.

(✓) 4. Standard Calibration Check standard 0. 100 AC
Result: 0. 096 AC

Instrument is operating properly and accurately. YES NO

COMMENTS None.

SIGNATURE Clare Conley

INTOXILYZER 8000
Location: ARIZONA
Serial Number : 80-002201
08/28/2008

12:15:18

207
cu
py

Standard Lot#: 735401G
Last Changed By: J. OLIVARES #36552

QAS: C. CONLEY #34517
TUCSON PD

Operator: C. CONLEY #34517
TUCSON PD

Subject: TEST, SQAP
DOB: 11/11/1111
Sex: M Weight: 111

15 Minute Deprivation Period? Yes

Test	g/210L	Time
Air Blank	0.000	12:16:18
Diagnostic Test	Pass	12:16:46
Air Blank	0.000	12:17:13
0.100 Cal Check	0.097	12:17:32
Air Blank	0.000	12:18:01
Subject Test	0.000	12:18:21
Air Blank	ABT*	12:18:27
Air Blank	0.000	12:18:56

*Sequence Aborted

Not a Successfully Completed Test Sequence

INTOXILYZER 8000
Location: ARIZONA
Serial Number : 80-002201
08/28/2008

12:19:02

3567
cu
134

Standard Lot#: 735401G
Last Changed By: J. OLIVARES #36552

QAS: C. CONLEY #34517
TUCSON PD

Operator: C. CONLEY #34517
TUCSON PD

Subject: TEST, SQAP
DOB: 11/11/1111
Sex: M Weight: 111

15 Minute Deprivation Period? Yes

Test	g/210L	Time
Air Blank	RFI*	12:19:36
Air Blank	IPS**	12:19:45

*RFI Detect
**Improper Sample

Not a Successfully Completed Test Sequence

INTOXILYZER 8000
Location: ARIZONA
Serial Number : 80-002201
08/28/2008

12:19:50

Standard Lot#: 735401G
Last Changed By: J. OLIVARES #36552

QAS: C. CONLEY #34517
TUCSON PD

Operator: C. CONLEY #34517
TUCSON PD

Subject: TEST, SQAP
DOB: 11/11/1111
Sex: M Weight: 111

15 Minute Deprivation Period? Yes

4567
cu
184

Test	g/210L	Time
Air Blank	0.000	12:20:44
Diagnostic Test	Pass	12:21:11
Air Blank	0.000	12:21:39
0.100 Cal Check	0.098	12:21:57
Air Blank	0.000	12:22:27
Subject Test	0.247*	12:25:35
Air Blank	0.000	12:26:08
Air Blank	0.000	12:26:35
Subject Test	XXX**	12:26:59
Air Blank	0.000	12:27:32

*Deficient Sample

**Invalid Sample

Begin new deprivation period

Not a Successfully Completed Test Sequence

INTOXILYZER 8000
Location: ARIZONA
Serial Number: 80-002201
08/28/2008

12:27:52

Standard Lot#: 735401G
Last Changed By: J. OLIVARES #36552

QAS: C. CONLEY #34517
TUCSON PD

Test	g/210L	Time
Air Blank	0.000	12:28:19
Cal Check	0.096	12:28:38
Air Blank	0.000	12:29:08

Claire Conley
Operator's Signature

5007
cu
12/4

EXHIBIT G-2

THIS REPORT PREPARED PURSUANT TO DUTY IMPOSED BY
A.A.C. R13-10-104(A)

ARIZONA DEPARTMENT OF PUBLIC SAFETY

STANDARD QUALITY ASSURANCE PROCEDURES
INTOXILYZER MODEL 8000

STANDARD CALIBRATION CHECK PROCEDURE

6567
Cu

BY
8-29-08

QA Specialist Clare Conley AGENCY Tucson Police Department
DATE 8-28-08 TIME 1213
Intoxilyzer Serial # 80-002201 Location Vehicle #817

- (✓) 1. Ensure that gas tank is attached to instrument and contains a standard alcohol concentration solution 0. 100 AC.
OR
Pour a standard alcohol concentration solution _____ AC, into a clean dry simulator and assemble the simulator. Ensure that a tight seal has been made. Turn on the simulator and allow temperature to reach 34°C ± 0.2°C
- (✓) 2. Intoxilyzer 8000 display reads "PUSH BUTTON TO START"
- (✓) 3. Go to the "Control Testing Menu". Select "D" for dry control test or "W" for wet control test. After selection is made press ENTER.
- (✓) 4. Air blank completed.
- (✓) 5. Calibration check completed. Test results 0. 097 AC.
- (✓) 6. Air blank completed.
- (✓) 7. Remove printed record. Attach the record to the completed checklist.

SIGNATURE Clare Conley

DPS Form Exh G-2 (Rev. 05-01)

INTOXILYZER 8000
Location: ARIZONA
Serial Number: 80-002201
08/28/2008

12:13:57

Standard Lot#: 735401G
Last Changed By: J. OLIVARES #36552

QAS: C. CONLEY #34517
TUCSON PD

Test	g/210L	Time
Air Blank	0.000	12:14:24
Cal Check	0.097	12:14:43
Air Blank	0.000	12:15:13

Clare Conley

Operator's Signature

7587
cu

154