



CERTIFICATION by CUSTODIAN of RECORDS
Tucson Police Department Crime Laboratory

I hereby certify that these documents are a true and correct copy of the periodic maintenance* for the Intoxilyzer 8000 Serial Number 80-002261 maintained by the Tucson Police Department Crime Laboratory pursuant to the requirements of the Arizona Department of Public Safety for a quality assurance program. ⁷⁵⁴

A quality assurance specialist (QAS) tested the instrument on the following dates. The acceptable accuracy limits, as defined in A.A.C. R13-10-104.A.2, for a 0.100AC solution are 0.090AC to 0.110AC.


Date: 12/1/06 Cal 1 0.098 AC Cal 2 0.100 AC

The instrument was placed into service on 12/1/06.

Jennifer L. Coombs
Jennifer L. Coombs
12/27/06

ADPS QAS Permit # 33120

SUBSCRIBED AND SWORN to before me this 27, day of December, 2006.

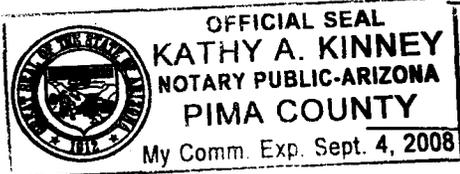

Kathy A. Kinney
Notary Public

*Includes documents specified in A.A.C. R13-10-104.A.5

THIS REPORT PREPARED PURSUANT TO DUTY IMPOSED BY
A.A.C. R13-10-104 (A)

1 of 8
file

ARIZONA DEPARTMENT OF PUBLIC SAFETY
STANDARD QUALITY ASSURANCE PROCEDURES
INTOXILYZER MODEL 8000
STANDARD QUALITY ASSURANCE PROCEDURE

TH

QA SPECIALIST Jennifer Coombs 46660 AGENCY Tucson Police Department
DATE December 1, 2006 TIME 11008
INTOXILYZER SERIAL # 80-002261 LOCATION LAB

(✓) 1. Display reads "PUSH BUTTON TO START"

DIAGNOSTIC TESTS

- (✓) 1. Clock time check.
- (✓) 2. Date check.

OPERATIONAL TESTS

- (✓) 1. Alcohol-free subject test result 0. 000 AC.
- (✓) 2. Error recognition logic system functioning.
Not a Successfully Completed Test Sequence printed ✓✓✓
- (✓) 3. Proper sample recognition system.
Not a Successfully Completed Test Sequence printed
Deficient sample printed.
- (✓) 4. Standard Calibration Check standard 0. 100 AC
Result: 0. 098 AC

Instrument is operating properly and accurately. YES NO

COMMENTS

SIGNATURE Jennifer L. Coombs

Pursuant to section 28-1327, Arizona Revised Statutes, this document is a certified duplicate of the information contained in computer storage devices of the Tucson Police Department.

INTOXILYZER 8000
Location: TUCSON POLICE DEPT
Serial Number : 80-002261
12/01/2006

16:09:30

24

2 of 8
file

Standard Lot#: 502602I
Last Changed By: J. COOMBS #46160

QAS: J. COOMBS #46160
TUCSON PD CRIME LAB

Operator: J. COOMBS #46160
TUCSON PD CRIME LAB

Subject: SQAP, TEST
DOB: 11/11/1111
Sex: F Weight: 111

15 Minute Deprivation Period? Yes

Test	g/210L	Time
Air Blank	0.000	16:10:27
Diagnostic Test	Pass	16:10:54
Air Blank	0.000	16:11:22
0.100 Cal Check	0.099	16:11:40
Air Blank	0.000	16:12:10
Subject Test	0.000	16:12:55
Air Blank	0.000	16:13:23
Five Minute Wait	ABT*	
Air Blank	0.000	16:14:04

*Sequence Aborted

Not a Successfully Completed Test Sequence

INTOXILYZER 8000
Location: TUCSON POLICE DEPT
Serial Number : 80-002261
12/01/2006

16:14:16

TM

3 of 8
file

Standard Lot#: 502602I
Last Changed By: J. COOMBS #46160

QAS: J. COOMBS #46160
TUCSON PD CRIME LAB

Operator: J. COOMBS #46160
TUCSON PD CRIME LAB

Subject: SQAP, TEST
DOB: 11/11/1111
Sex: F Weight: 111

15 Minute Deprivation Period? Yes

Test	g/210L	Time
Air Blank	IPS*	16:14:54
Air Blank	0.000	16:15:23

*Improper Sample

Not a Successfully Completed Test Sequence

INTOXILYZER 8000
Location: TUCSON POLICE DEPT
Serial Number : 80-002261
12/01/2006

16:15:39

PH

4 of 8
file

Standard Lot#: 502602I
Last Changed By: J. COOMBS #46160

QAS: J. COOMBS #46160
TUCSON PD CRIME LAB

Operator: J. COOMBS #46160
TUCSON PD CRIME LAB

Subject: SQAP, TEST
DOB: 11/11/1111
Sex: F Weight: 111

15 Minute Deprivation Period? Yes

Test	g/210L	Time
Air Blank	0.000	16:16:43
Diagnostic Test	Pass	16:17:10
Air Blank	0.000	16:17:38
0.100 Cal Check	RFI*	16:17:55
Air Blank	0.000	16:18:26

*RFI Detect

Not a Successfully Completed Test Sequence

INTOXILYZER 8000
Location: TUCSON POLICE DEPT
Serial Number : 80-002261
12/01/2006

16:22:04

ph

5 of 8
file

Standard Lot#: 502602I
Last Changed By: J. COOMBS #46160

QAS: J. COOMBS #46160
TUCSON PD CRIME LAB

Operator: J. COOMBS #46160
TUCSON PD CRIME LAB

Subject: SQAP,TEST
DOB: 11/11/1111
Sex: F Weight: 111

15 Minute Deprivation Period? Yes

Test	g/210L	Time
Air Blank	0.000	16:22:59
Diagnostic Test	Pass	16:23:27
Air Blank	0.000	16:23:54
0.100 Cal Check	0.099	16:24:13
Air Blank	0.000	16:24:42
Subject Test	0.028*	16:27:51
Air Blank	0.000	16:28:22
Air Blank	0.000	16:28:49
Subject Test	XXX**	16:29:05
Air Blank	0.000	16:29:39

*Deficient Sample

**Invalid Sample

Begin new deprivation period

Not a Successfully Completed Test Sequence

INTOXILYZER 8000

Location: TUCSON POLICE DEPT

Serial Number: 80-002261

12/01/2006

16:29:59

B4

leaf 8
file


Standard Lot#: 502602I

Last Changed By: J. COOMBS #46160

QAS: J. COOMBS #46160

TUCSON PD CRIME LAB

Test	g/210L	Time
Air Blank	0.000	16:30:26
Cal Check	0.098	16:30:45
Air Blank	0.000	16:31:15

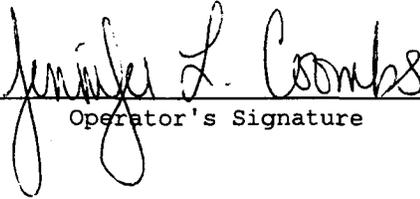

Operator's Signature

THIS REPORT PREPARED PURSUANT TO DUTY IMPOSED BY
A.A.C. R13-10-104(A)

7 of 8
file

ARIZONA DEPARTMENT OF PUBLIC SAFETY

STANDARD QUALITY ASSURANCE PROCEDURES
INTOXILYZER MODEL 8000

bu

STANDARD CALIBRATION CHECK PROCEDURE

QA Specialist Jennifer Coombs 416160 AGENCY Tucson Police Department
DATE December 1, 2006 TIME 11:08
Intoxilyzer Serial # 80-002261 Location LAB

- (✓) 1. Ensure that gas tank is attached to instrument and contains a standard alcohol concentration solution 0. 100 AC.
OR
Pour a standard alcohol concentration solution _____ AC, into a clean dry simulator and assemble the simulator. Ensure that a tight seal has been made. Turn on the simulator and allow temperature to reach 34°C ± 0.2°C
- (✓) 2. Intoxilyzer 8000 display reads "PUSH BUTTON TO START"
- (✓) 3. Go to the "Control Testing Menu". Select "D" for dry control test or "W" for wet control test. After selection is made press ENTER.
- (✓) 4. Air blank completed.
- (✓) 5. Calibration check completed. Test results 0. 100 AC.
- (✓) 6. Air blank completed.
- (✓) 7. Remove printed record. Attach the record to the completed checklist.

SIGNATURE Jennifer L. Coombs

Pursuant to section 28-1327, Arizona Revised Statutes, this document is a certified duplicate of the information contained in computer storage devices of the Tucson Police Department.

INTOXILYZER 8000

Location: TUCSON POLICE DEPT

Serial Number: 80-002261

12/01/2006

16:08:05

126

8 of 8
file


Standard Lot#: 502602I

Last Changed By: J. COOMBS #46160

QAS: J. COOMBS #46160

TUCSON PD CRIME LAB

Test	g/210L	Time
Air Blank	0.000	16:08:33
Cal Check	0.100	16:08:52
Air Blank	0.000	16:09:21

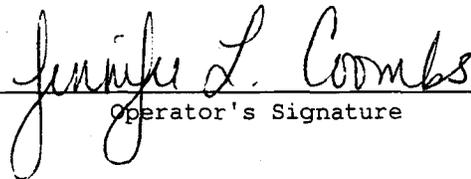
Operator's Signature



TUCSON POLICE DEPARTMENT
CRIME LABORATORY

INTOXILYZER SERVICE RECORD

1 of 1
file

754

Intoxilyzer Serial Number: 80-002261

Initial Service Date: 12-1-06

CMI, Inc. Certificate of Calibration Date: 11-10-06